



## Series EXP-SNR-TG-EC-ITS-ALG

### Explosion Proof Carbon Dioxide Sensor

---

#### **US Office**

Larson Electronics, LLC.  
9419 US-HWY 175  
Kemp, TX 75143

Ph: 800-369-6671  
903-498-3363

Fax: 903-498-3364

Email: [sales@larsonelectronics.com](mailto:sales@larsonelectronics.com)

---

# Table of Contents



|                                                                           |           |
|---------------------------------------------------------------------------|-----------|
| <b>INTRODUCTION .....</b>                                                 | <b>5</b>  |
| IR GAS SENSOR.....                                                        | 5         |
| IR SENSOR VERSIONS .....                                                  | 7         |
| STANDARD LEL HYDROCARBON (HC) IR SENSOR, P/N 00-1375 .....                | 7         |
| LEL, UEL.....                                                             | 9         |
| %LEL .....                                                                | 9         |
| Target and Interferent Gases .....                                        | 9         |
| Managing Interferent Gas Environments.....                                | 9         |
| Methane and High-Methane Target Gas Settings... ..                        | 10        |
| HIGH-RANGE HYDROCARBON (HHC) IR SENSOR, P/N 00-1376 .....                 | 11        |
| STANDARD RANGE CARBON DIOXIDE (CO2) IR SENSOR, 0-5%VOL, P/N 00-1377 ..... | 11        |
| HIGH-RANGE CARBON DIOXIDE (HCO2) IR SENSOR, 0-50%VOL,P/N 00-1378 .....    | 12        |
| STANDARD RANGE NITROUS OXIDE (N2O) IR SENSOR, 0-1%VOL , P/N 00-1431 ..... | 12        |
| <b>SPECIFICATIONS .....</b>                                               | <b>13</b> |
| <b>INSTALLATION.....</b>                                                  | <b>14</b> |
| HAZARDOUS LOCATIONS .....                                                 | 14        |
| MECHANICAL MOUNTING.....                                                  | 15        |
| Supporting the Transmitter .....                                          | 15        |
| ELECTRICAL CONNECTIONS.....                                               | 16        |
| External Power Supply.....                                                | 16        |
| The Stack.....                                                            | 16        |
| Power Supply Board .....                                                  | 17        |
| Relay Contacts .....                                                      | 18        |
| Wiring Examples .....                                                     | 19        |
| A17/B14, 3-Wire Mode.....                                                 | 19        |
| Power Without 4-20mA Signaling .....                                      | 20        |
| 4-20mA Signaling, Single Supply, 3-Wire Mode .....                        | 21        |
| 4-20mA Signaling, Dual Supply, 4-Wire Mode .....                          | 22        |
| HART Transmitter, Point-to-Point, 3-Wire (Active Source) .....            | 23        |
| HART Transmitter, Multi-drop, 3-Wire (Active Source) .....                | 24        |
| RS485 Modbus Multidrop.....                                               | 25        |
| RS232 Modbus, PC Capture, or Printer .....                                | 26        |
| REMOTE SENSOR WIRING .....                                                | 27        |
| CPU Board Configuration.....                                              | 28        |
| <b>OPERATION .....</b>                                                    | <b>30</b> |
| Interface Panel.....                                                      | 30        |
| Startup Review Sequence .....                                             | 31        |
| Main Display Page.....                                                    | 32        |

|                                                           |           |
|-----------------------------------------------------------|-----------|
| Five-minute Time-out Rule .....                           | 32        |
| Esc Key Operation - Main Display Only .....               | 32        |
| Fault Indication.....                                     | 32        |
| Main Reading .....                                        | 33        |
| Menu Page .....                                           | 33        |
| Setup Page .....                                          | 33        |
| Variable Editing.....                                     | 34        |
| <b>SENSORS.....</b>                                       | <b>35</b> |
| Sensor Setup Pages .....                                  | 35        |
| Sensor Target Gas, Range, Units, and LEL Variables .....  | 35        |
| Sensor Damping, Blanking, and Temperature Variables ..... | 36        |
| Sensor Cal History (Link).....                            | 36        |
| Bump-Testing .....                                        | 37        |
| Calibration .....                                         | 38        |
| Calibration Frequency .....                               | 38        |
| Calibration Terminology .....                             | 38        |
| Zero Calibration.....                                     | 38        |
| Span Calibration .....                                    | 38        |
| Calibration Kits .....                                    | 38        |
| Indications During Sensor Calibration.....                | 38        |
| Calibration Exceptions.....                               | 38        |
| Zero Calibration with a Zero Gas Source .....             | 39        |
| Zeroing to the Atmosphere .....                           | 39        |
| Zero Sensor Page .....                                    | 39        |
| Span Calibration Procedure .....                          | 40        |
| Spanning for Safety – HC and HHC IR Sensors.....          | 41        |
| Sensor Calibration Records .....                          | 42        |
| <b>ALARMS AND RELAYS.....</b>                             | <b>43</b> |
| Gas Concentration Alarms.....                             | 43        |
| Manual Alarm Reset.....                                   | 43        |
| Remote Reset.....                                         | 43        |
| Gas Alarm Setup Pages .....                               | 44        |
| Alarm Variable Functions.....                             | 47        |
| Fault Alarms.....                                         | 48        |
| Corrective Actions.....                                   | 48        |
| Alarm Relays .....                                        | 51        |
| Relay Setup Page .....                                    | 52        |
| Testing Alarm Relays .....                                | 52        |
| Relay Test Page.....                                      | 52        |
| Inhibiting Alarms.....                                    | 53        |
| Alarm Inhibit Setup page.....                             | 53        |
| <b>4-20MA ANALOG OUTPUT .....</b>                         | <b>54</b> |
| Output Overrides .....                                    | 54        |
| 4-20mA Setup Page .....                                   | 54        |
| 4-20mA Control Page.....                                  | 55        |
| Loop Adjustment .....                                     | 55        |
| <b>DATA LOGGER .....</b>                                  | <b>56</b> |
| Data-log Access Page .....                                | 57        |
| Data-log Setup Page .....                                 | 57        |
| Data-log Graphic Report Page .....                        | 58        |
| Data-log Tabular Report Page .....                        | 58        |
| Data-log Printout .....                                   | 59        |
| <b>DISPLAY .....</b>                                      | <b>60</b> |
| Display Setup Page.....                                   | 60        |
| <b>SYSTEM .....</b>                                       | <b>61</b> |
| System Access Page .....                                  | 61        |
| Real-time Clock.....                                      | 61        |
| Clock Setup Page.....                                     | 61        |

## **Series EXP-SNR Gas Transmitter with IR Sensor**


|                                  |           |                                            |    |
|----------------------------------|-----------|--------------------------------------------|----|
| <i>Security</i> .....            | 62        | PRINTING DATA LOG REPORTS .....            | 70 |
| Security Control Page.....       | 62        | <i>Serial Connection</i> .....             | 70 |
| Activating Security.....         | 62        | <i>Communication Setup Page</i> .....      | 70 |
| Deactivating Security.....       | 63        | <i>Flow Control</i> .....                  | 70 |
| Changing the Password .....      | 63        | <i>Report Format</i> .....                 | 71 |
| <i>Communications</i> .....      | 64        | <i>Report Control</i> .....                | 71 |
| Communication Setup Page .....   | 64        | EXAMPLE: CHARTING A DATA LOG REPORT .....  | 72 |
| ASCII.....                       | 65        | <i>Starting the Report</i> .....           | 75 |
| HART.....                        | 65        | <i>Charting with Microsoft Excel</i> ..... | 78 |
| Modbus .....                     | 67        |                                            |    |
| <i>Transmitter Version</i> ..... | 67        |                                            |    |
| <i>Restart</i> .....             | 68        |                                            |    |
| <i>Resets</i> .....              | 68        |                                            |    |
| <b>SPARE PARTS</b> .....         | <b>69</b> |                                            |    |
| <b>APPENDIX A</b> .....          | <b>70</b> |                                            |    |

## **List of Figures**


|                                                               |    |                                                            |    |
|---------------------------------------------------------------|----|------------------------------------------------------------|----|
| FIGURE 1. EXP-SNR TRANSMITTER .....                           | 5  | FIGURE 38. RISING ALARM (ACTIVE=ABOVE_SP, RESET=AUTO) 47   |    |
| FIGURE 2. IR GAS SENSOR. ....                                 | 5  | FIGURE 39. FALLING ALARM (ACTIVE=BELOW_SP, RESET=AUTO)     |    |
| FIGURE 3. SIGNAL OUTPUTS WITH AND WITHOUT GAS EXPOSURE.....   | 5  | .....                                                      | 47 |
| FIGURE 4. ABSORPTION SPECTRUM AND SENSOR RESPONSE.....        | 6  | FIGURE 40. FAULT ALARM (MAIN DISPLAY) .....                | 48 |
| FIGURE 5. COMPARISON OF "METHANE" TO "HIGH-METHANE"           |    | FIGURE 41. FAULT PAGE .....                                | 48 |
| LINEARIZATION FOR LOW CONCENTRATIONS .....                    | 10 | FIGURE 42 ALARM RELAY SCHEMATIC .....                      | 51 |
| FIGURE 6. COMPARISON OF "METHANE" TO "HIGH-METHANE"           |    | FIGURE 43. RELAY SETUP PAGE (EXAMPLE) .....                | 52 |
| LINEARIZATION FOR HIGH CONCENTRATIONS.....                    | 10 | FIGURE 44. RELAY TEST PAGE EXAMPLE.....                    | 52 |
| FIGURE 7. OVERALL DIMENSIONS .....                            | 15 | FIGURE 45. INHIBITING ALARMS FROM THE MAIN DISPLAY.....    | 53 |
| FIGURE 8. ACCESSING ELECTRICAL CONNECTIONS .....              | 16 | FIGURE 46. ALARM INHIBIT SETUP PAGE .....                  | 53 |
| FIGURE 9. POWER SUPPLY BOARD CONNECTIONS.....                 | 17 | FIGURE 47. CURRENT LOOP OUTPUT PLOT.....                   | 54 |
| FIGURE 10. RELAY CONTACTS.....                                | 18 | FIGURE 48. 4-20mA SETUP PAGE .....                         | 54 |
| FIGURE 11. A17/B14 EXAMPLE.....                               | 19 | FIGURE 49. 4-20mA CONTROL PAGE .....                       | 55 |
| FIGURE 12. POWER WITHOUT 4-20mA SIGNALING EXAMPLE .....       | 20 | FIGURE 50. LOOP ADJUSTMENT PAGES.....                      | 55 |
| FIGURE 13. 4-20mA SIGNALING, SINGLE SUPPLY, 3-WIRE EXAMPLE    |    | FIGURE 51. DATA LOG ACCESS PAGE .....                      | 57 |
| .....                                                         | 21 | FIGURE 52. DATA LOG SETUP PAGE .....                       | 57 |
| FIGURE 14. 4-20mA SIGNALING, DUAL SUPPLY, 4-WIRE EXAMPLE..    | 22 | FIGURE 53. DATA LOG GRAPHIC REPORT PAGE.....               | 58 |
| FIGURE 15. HART TRANSMITTER, POINT-TO-POINT, 3-WIRE           |    | FIGURE 54. DATA LOG TABULAR REPORT PAGE.....               | 58 |
| EXAMPLE .....                                                 | 23 | FIGURE 55. DATA-LOG PRINTOUT.....                          | 59 |
| FIGURE 16. HART TRANSMITTER, MULTI-DROP, 3-WIRE EXAMPLE.      | 24 | FIGURE 56. SYSTEM ACCESS PAGE .....                        | 61 |
| FIGURE 17. RS485 MODBUS MULTIDROP EXAMPLE .....               | 25 | FIGURE 57. CLOCK SETUP PAGE .....                          | 61 |
| FIGURE 18. RS232 MODBUS, PC CAPTURE, PRINTER EXAMPLE ....     | 26 | FIGURE 58. SECURITY CONTROL PAGE .....                     | 62 |
| FIGURE 19. REMOTE SENSOR OPTION WIRING.....                   | 27 | FIGURE 59. ACTIVATING SECURITY.....                        | 62 |
| FIGURE 20. CPU BOARD CONFIGURATION .....                      | 28 | FIGURE 60. DEACTIVATING SECURITY .....                     | 63 |
| FIGURE 21. OPERATORS INTERFACE PANEL .....                    | 30 | FIGURE 61. CHANGING THE PASSWORD.....                      | 63 |
| FIGURE 22. STARTUP REVIEW SEQUENCE.....                       | 31 | FIGURE 62. COMMUNICATION SETUP PAGE .....                  | 64 |
| FIGURE 23. MAIN DISPLAY .....                                 | 32 | FIGURE 63. HART SETUP PAGES .....                          | 65 |
| FIGURE 24. MENU AND SETUP PAGES.....                          | 33 | FIGURE 64. HART A) FIND-ME AND B) DEVICE FOUND PAGES ..... | 66 |
| FIGURE 25. VARIABLE EDITING .....                             | 34 | FIGURE 65. MODBUS SETUP PAGE .....                         | 67 |
| FIGURE 26. SENSOR SETUP AND GAS/RANGE/UNITS PAGES .....       | 35 | FIGURE 66. TRANSMITTER VERSION PAGE.....                   | 67 |
| FIGURE 27. DATA-LOG WARNING PAGE .....                        | 35 |                                                            |    |
| FIGURE 28. SENSOR SETUP AND DAMP/BLANK/TEMP SETUP PAGE...36   |    |                                                            |    |
| FIGURE 29. SENSOR CAL HISTORY (LINK) .....                    | 36 |                                                            |    |
| FIGURE 30. ZERO CALIBRATION.....                              | 39 |                                                            |    |
| FIGURE 31. ZERO_SENSOR PAGE .....                             | 39 |                                                            |    |
| FIGURE 32. SPAN CALIBRATION .....                             | 40 |                                                            |    |
| FIGURE 33. SPAN_SENSOR PAGE .....                             | 40 |                                                            |    |
| FIGURE 34. SENSOR CALIBRATION HISTORY PAGES .....             | 42 |                                                            |    |
| FIGURE 35. DEFAULT ALARMS FOR COMBUSTIBLE GAS SENSORS. ....43 |    |                                                            |    |
| FIGURE 36. MANUAL ALARM RESET.....                            | 43 |                                                            |    |
| FIGURE 37. ALARM SETUP PAGES (EXAMPLE) .....                  | 44 |                                                            |    |

## INTRODUCTION

The EXP-SNR transmitter is used to continuously monitor for gas leaks in ambient air near process tanks, piping, or in enclosed spaces where gases may accumulate. The transmitter is explosion proof, and is rated for use in hazardous locations (see specifications). It features an NDIR (non-dispersive, infrared) sensor, a non-intrusive four button user interface with a back-lighted graphics display, three level alarm system with three (optional) alarm relays, high-resolution 4-20mA current loop output, real-time clock, data-logger, and optional HART™ or Modbus™ network interface.

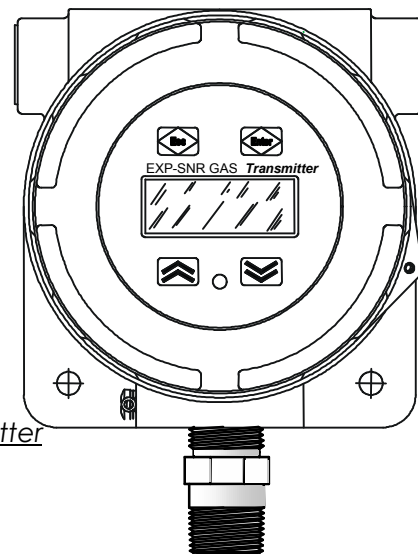

*Figure 1. EXP-SNR transmitter*

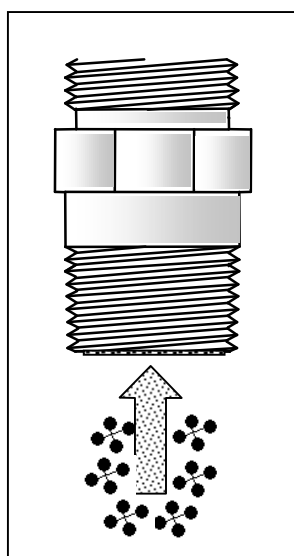


### IR Gas Sensor

The IR sensor is housed in an explosion proof, stainless steel housing that is threaded into the base of the transmitter (or remote housing, if ordered). A porous, stainless steel frit is welded into the opposite end to permit gas entry, and to prevent possible ignition of a combustible atmosphere. Threads are cut into the sensor housing to accommodate various accessories, such as rain shields, and calibration adapters.

The working parts of the sensor consist of an infrared light source, detector, thermistor, and memory device. The light source is a thin wall, tungsten filament lamp, with an MTBF of over 5 years. It is pulsed at 2 Hz to provide excitation to the detector, and as a side benefit, warms the components of the sensor. This helps to prevent water vapor from condensing on the interior surfaces of the sensor, which could lead to excessive drift, or even false alarms.

*Figure 2. IR gas sensor.*


The detector is a dual element, pyroelectric design. The elements, labeled “active” and “reference”, are piezo crystals that distort when heated, and generate a small charge in response to radiation pulses emitted by the lamp. Specially designed, optical filters cover each element. The active element is covered by an optical filter that passes radiation in a band that will be absorbed by a target gas, such as Methane. Its output will decrease in amplitude when the gas is in the path of the lamp’s radiation. The “reference” element has an optical filter whose pass-band is outside of the active element’s filter, and is unaffected by the presence of the target gas. It is used primarily to compensate for slight variations of lamp intensity, humidity, and other environmental factors.

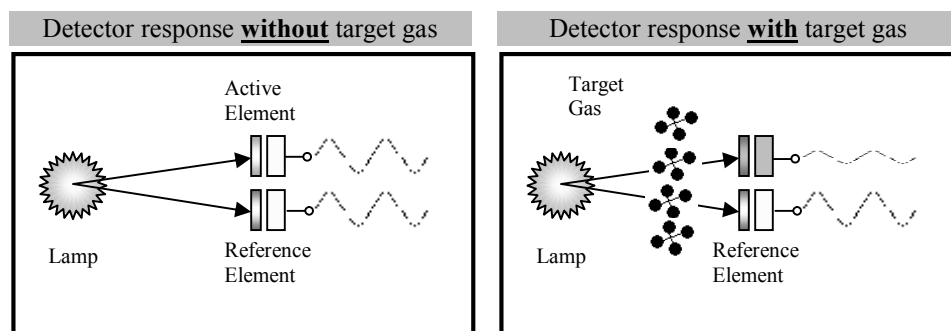

*Figure 3. Signal outputs with and without gas exposure.*

### Series EXP-SNR Gas Transmitter with IR Sensor

The signal output of an element is proportional to the amount of filtered radiation reaching it. When an IR absorbing gas enters the optical path, it reduces the radiation reaching the active element by an amount that is a function of the gas type, and concentration. The figure below illustrates the absorption spectra of both Methane and Propane at identical concentrations, overlaid with the filter pass-bands of the Standard LEL Hydrocarbon sensor (P/N 00-1375). To the right of each spectrum is a graph of the sensor's relative, fractional absorption (FA) plotted over the same concentration range.

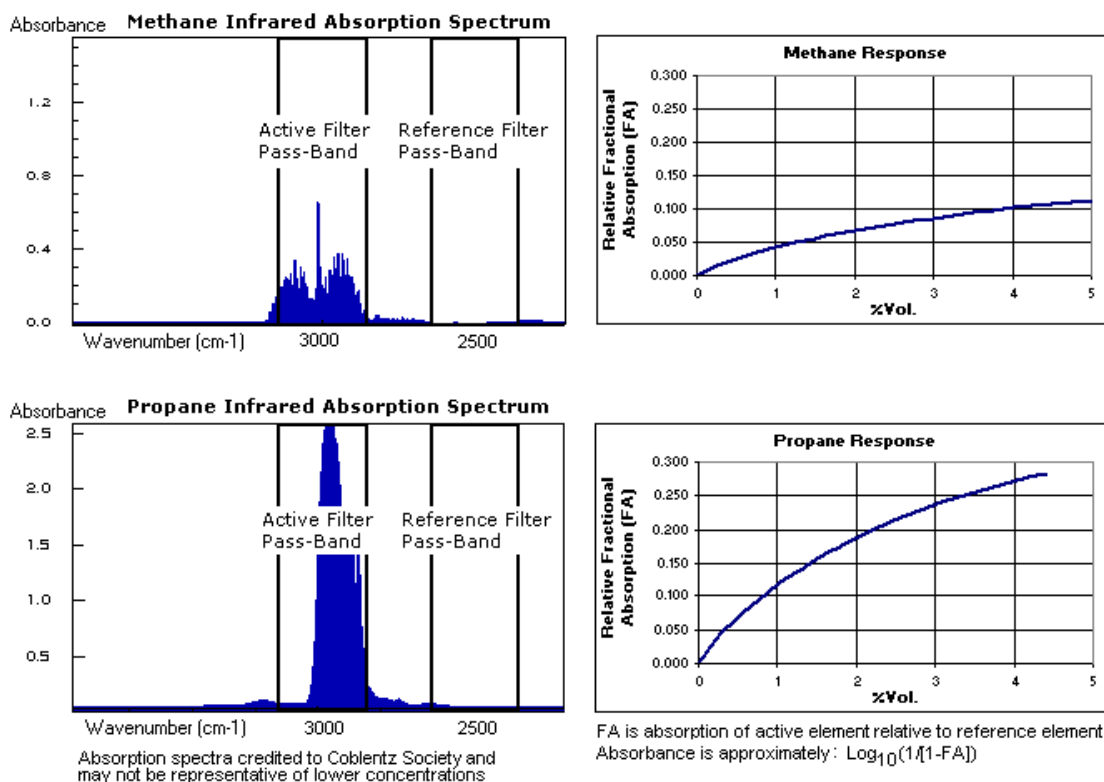

*Figure 4. Absorption spectrum and sensor response*

The transmitter's CPU monitors the output from each element, computes a fractional absorption value and linearizes it into a gas concentration reading in units of %LEL, or %V/V. The linearization function is derived from Beer's Law. The CPU also monitors the sensor's thermistor output and, if required, corrects the concentration readings over its specified temperature range.

The memory of the sensor stores a table of information about one or more target gasses, including names, ranges, alarm settings, linearity, sensitivity, and calibration status information. Once the factory has calibrated the sensor with one or more gasses listed in the table, any one of those gasses may be selected for monitoring at the customer site. In addition to the gas table, the sensor memory stores a calibration history. The history includes room for 63 zero, and 63 span calibration records, before rolling over.

## IR Sensor Versions

**Table 1. IR sensor versions.**

| Part No. | Abbreviation | Description                                                                                             |
|----------|--------------|---------------------------------------------------------------------------------------------------------|
| 00-1375  | HC           | Standard LEL (low range) hydrocarbon sensor for Methane, Propane, Butane, Pentane, etc.                 |
| 00-1376  | HHC          | High range hydrocarbon sensor for high concentrations (normally above the UEL) of Propane, Butane, LPG. |
| 00-1377  | CO2          | Standard range Carbon dioxide sensor                                                                    |
| 00-1378  | HCO2         | High range Carbon dioxide sensor                                                                        |
| 00-1431  | N2O          | Standard range Nitrous oxide sensor                                                                     |

**Sensors are not approved for monitoring Acetylene.**

## Standard LEL Hydrocarbon (HC) IR Sensor, P/N 00-1375

**Table 2.**

**Target gas settings for the standard LEL hydrocarbon IR sensor**

The HC version of the IR sensor is designed to detect leaks of Methane, Propane, Butane, and other combustible gasses.

With so many potentially explosive, hydrocarbon gasses in use today, this sensor has the largest table of target gases. Each gas must be span calibrated at the factory to permit its selection in the field.

| Target Gas Setting                                                                                                                                                                                                                                                                                                                                  | LEL %V/Air | UEL * %V/Air | Default FS Range %LEL | Default Caution %LEL | Default Warning %LEL | Default Alarm %LEL | FA% @LEL |
|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|------------|--------------|-----------------------|----------------------|----------------------|--------------------|----------|
| Methane                                                                                                                                                                                                                                                                                                                                             | 5.0        | 15.0         | 100                   | -10 ▼                | 20 ▲                 | 50 ▲               | 11       |
| Ethane                                                                                                                                                                                                                                                                                                                                              | 3.0        | 12.4         | 100                   | -10 ▼                | 20 ▲                 | 50 ▲               | 10       |
| Propane                                                                                                                                                                                                                                                                                                                                             | 2.2        | 10.0         | 100                   | -10 ▼                | 20 ▲                 | 50 ▲               | 20       |
| n-Butane                                                                                                                                                                                                                                                                                                                                            | 1.8        | 9.0          | 100                   | -10 ▼                | 20 ▲                 | 50 ▲               | 19       |
| Pentane                                                                                                                                                                                                                                                                                                                                             | 1.5        | 7.8          | 100                   | -10 ▼                | 20 ▲                 | 50 ▲               | 16       |
| Hexane                                                                                                                                                                                                                                                                                                                                              | 1.2        | 7.4          | 100                   | -10 ▼                | 20 ▲                 | 50 ▲               | 13       |
| Cyclohexane                                                                                                                                                                                                                                                                                                                                         | 1.3        | 8.4          | 100                   | -10 ▼                | 20 ▲                 | 50 ▲               | 4        |
| Ethyl acetate                                                                                                                                                                                                                                                                                                                                       | 2.2        | 11.0         | 100                   | -10 ▼                | 20 ▲                 | 50 ▲               | 11       |
| Dimethyl - formamide (DMF)                                                                                                                                                                                                                                                                                                                          | 2.2        | 15.2         | 100                   | -10 ▼                | 20 ▲                 | 50 ▲               | 10       |
| Acetone                                                                                                                                                                                                                                                                                                                                             | 2.6        | 13.0         | 100                   | -10 ▼                | 20 ▲                 | 50 ▲               | 10       |
| Toluene                                                                                                                                                                                                                                                                                                                                             | 1.2        | 7.1          | 100                   | -10 ▼                | 20 ▲                 | 50 ▲               | 11       |
| Benzene                                                                                                                                                                                                                                                                                                                                             | 1.3        | 7.1          | 100                   | -10 ▼                | 20 ▲                 | 50 ▲               | 11       |
| High-Methane <sup>1</sup>                                                                                                                                                                                                                                                                                                                           | 5.0        | 15.0         |                       | Off                  | Off                  | Off                | ---      |
| Contact factory for complete list.<br>* Information only, HC sensor <b>not approved</b> for monitoring above LEL concentrations, except on High-Methane setting.<br><sup>1</sup> <b>Not approved</b> for monitoring concentrations at or below the LEL of any gas.<br>--- Not applicable, or not available at time of publication, contact factory. |            |              |                       |                      |                      |                    |          |

Unlike a catalytic bead sensor, compounds of Silicon do not poison the sensor, nor does it rely on atmospheric Oxygen. Although not entirely accurate above the target gas LEL, readings will not decrease when exposed to a

**Series EXP-SNR Gas Transmitter with IR Sensor**

100%Vol. concentration of the target gas. In addition, the sensor can operate in a 100%Vol. Methane environment (only on the High-Methane setting, see below).

## LEL, UEL

Various hydrocarbon gases become explosive when mixed with air at, or above, a concentration limit referred to as the LEL (Lower Explosive Limit). For Methane, the LEL concentration is 5% by volume, in air, labeled as 5%V/Air. As more gas is mixed with air, the concentration rises and remains explosive, until it reaches the UEL (Upper Explosive Limit). Above the UEL, the concentration is considered non-explosive. For Methane, the UEL concentration is 15%V/Air.

## %LEL

Various gas selections cause the transmitter to report combustible gas concentrations as a percentage of the LEL, or %LEL. For example, 2.5%V/Air of Methane would be reported as 50%LEL, and so on. A reading at or above 100%LEL indicates a dangerous, explosive environment exists at the transmitter, and every effort to evacuate personnel and prevent ignition should be taken.

By default, gasses listed in this sensor's table report concentration in units of %LEL, have alarms set at: C=-10, W=20 and A=50 %LEL, and are not permitted to have alarms set above 60%LEL (exception: High-Methane).

## Target and Interferent Gases

Any gas or vapor that absorbs IR in the pass-band of the active detector element will cause a positive response of the sensor. This principle permits a sensor to be used for monitoring more than one gas – but not at the same time. The IR sensor cannot distinguish one gas type from another, however; it can be calibrated for any gas that causes a positive response. Once calibrated (by the factory), that gas may be selected for monitoring at the customer site, and is referred to as a “target” gas. Once a target gas has been selected, any other gas that causes the sensor to respond (especially other target gases) is considered to be an “interferent” gas. Since the Standard LEL Hydrocarbon sensor has highest number of possible interferent gasses, a discussion of how to manage them appears below.

## Managing Interferent Gas Environments

As mentioned above, the Standard LEL Hydrocarbon sensor has the largest number of possible target gases, and since it may only monitor one at a time, it also has the largest number of possible interferent gases. In the best case, an interferent gas may cause nuisance alarms. In the worst case, it may pose an undetected, explosive, or deadly toxic atmosphere.


In locations where one or more IR absorbing gases may be present, select the target gas with the lowest FA (fractional absorption) at the LEL of the gas. This value is shown for most target gases in the table above as FA%@LEL. For example, consider the case where both Methane and Propane are piped through a confined space that must be monitored for potential leaks. The fractional absorption levels are found in table 2 above:

|         |     |      |     |      |     |     |     |
|---------|-----|------|-----|------|-----|-----|-----|
| Methane | 5.0 | 15.0 | 100 | -10▼ | 20▲ | 50▲ | 11  |
| Ethane  | 3.0 | 12.4 | 100 | -10▼ | 20▲ | 50▲ | --- |
| Propane | 2.2 | 10.0 | 100 | -10▼ | 20▲ | 50▲ | 20  |

In this case, Methane's 11 is less than the 20 for Propane, so we would select Methane as the target gas. If, by mistake, we were to make Propane the target gas, and subsequently experience a leak of Methane, the fractional absorption level would need to rise to 12.5 (the 50%LEL level of Propane) before triggering the alarm. A Methane leak would form an explosive mixture below that level, and therefore go undetected. Although a Propane leak might result in a false Methane alarm, the space would not be explosive.

### **Methane and High-Methane Target Gas Settings**

The sensor provides the “Methane”, and “High-Methane” settings to improve the accuracy of readings for low and high concentrations of Methane. As can be seen below, the “shape” of the sensor’s response at lower concentrations differs from that at higher concentrations, and the accuracy of readings can be improved by using a linearization function that more closely fits the response of the sensor.

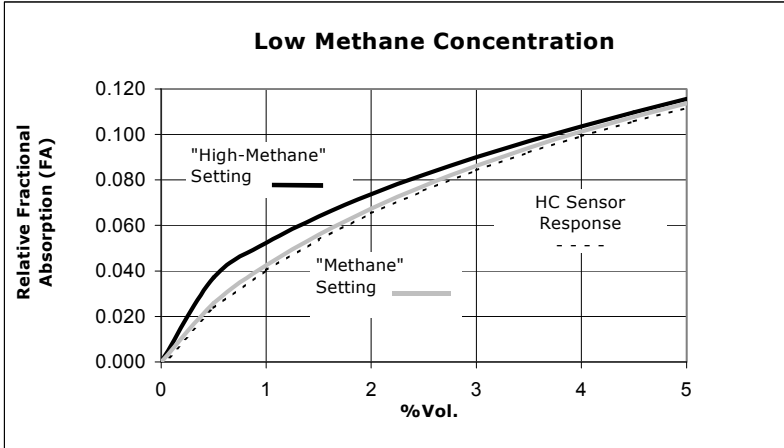


Choose the “Methane” setting when monitoring Methane concentrations below the LEL. This setting is typically used for detecting leaks in piping, and around storage tanks. This setting is not recommended for monitoring above the UEL (15%Vol).

*Figure 5. Comparison of "Methane" to "High-Methane" linearization for low concentrations*

Choose the “High-Methane” setting when monitoring Methane concentrations above the UEL (15%Vol.). This setting is typically used for process gas monitoring, or applications other than leak detection.

This setting is not recommended for monitoring below the LEL (5%Vol).

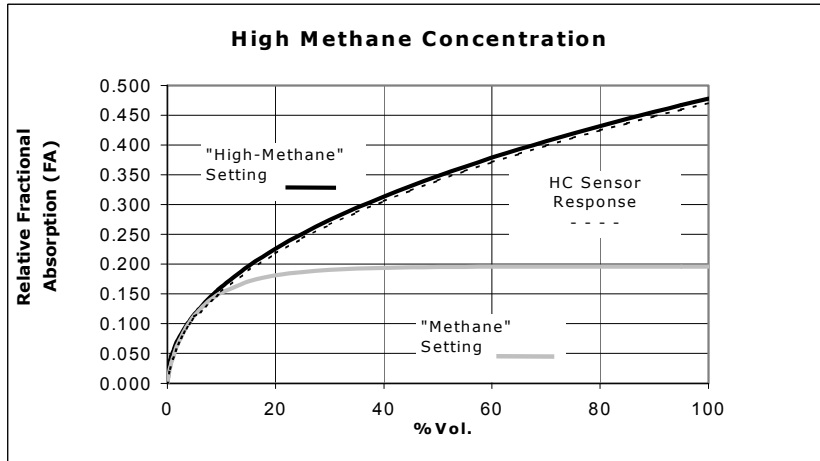

*Figure 6. Comparison of "Methane" to "High-Methane" linearization for high concentrations.*

### **High-range Hydrocarbon (HHC) IR Sensor, P/N 00-1376**

This version is designed to monitor high concentrations of hydrocarbon gas in locations where high concentrations are likely to exist normally, and usually above the UEL of the respective gas. Gases listed in this sensor's table include Propane, n-Butane, and LPG. Each gas must be span calibrated at the factory to permit its selection in the field. This sensor is **not recommended** for Methane, and is **not recommended** for monitoring concentrations at or below the LEL of any gas. For these applications, please use P/N 00-1375, Standard LEL Hydrocarbon IR Sensor.

**Table 3. Target gas settings for the High-range Hydrocarbon IR Sensor**

| Target Gas Setting                                                                                                                 | FS Range (Min,Max)   | Default Caution | Default Warning | Default Alarm |
|------------------------------------------------------------------------------------------------------------------------------------|----------------------|-----------------|-----------------|---------------|
| Propane                                                                                                                            | 100 %V/V<br>(10,100) | Off             | Off             | Off           |
| n-Butane                                                                                                                           | 100 %V/V<br>(10,100) | Off             | Off             | Off           |
| LPG                                                                                                                                | 100 %V/V<br>(10,100) | Off             | Off             | Off           |
| Contact factory for complete list.<br>HHC sensor <b>not approved</b> for monitoring concentrations at or below the LEL of any gas. |                      |                 |                 |               |

By default, gasses listed in this sensor's table report concentration in units of %V/V (equivalent to %V/Air, or %Vol), and have their alarms disabled. Alarms may be enabled, and programmed to activate on either rising or falling concentration levels.

### **Standard range Carbon Dioxide (CO2) IR Sensor, 0-5%Vol, P/N 00-1377**

**Table 4. Target gas settings for the Standard-range Carbon Dioxide IR Sensor**

| Target Gas Setting                 | FS Range (Min,Max)      | Default Caution | Default Warning | Default Alarm |
|------------------------------------|-------------------------|-----------------|-----------------|---------------|
| CO2                                | 1.0 %V/V<br>(1.0,5.0)   | -0.1 %V/V ▼     | 0.2 %V/V ▲      | 0.5 %V/V ▲    |
| Low-CO2                            | 2000 PPM<br>(2000,5000) | -200 PPM ▼      | 2000 PPM ▲      | 5000 PPM ▲    |
| Contact factory for complete list. |                         |                 |                 |               |

This version provides a "CO2", and "Low-CO2" setting to improve the accuracy of readings for high and low concentrations of Carbon dioxide. The "shape" of the sensor's response at lower concentrations differs from that at higher concentrations, and the accuracy of readings are improved by using the linearization that more closely fits the response of the sensor.

## **High-range Carbon Dioxide (HCO<sub>2</sub>) IR Sensor, 0-50%Vol,P/N 00-1378**

**Table 5. Target gas settings for the High-range CO<sub>2</sub> IR Sensor**

| <b>Target Gas Setting</b>                                                                                                             | <b>FS Range (Min,Max)</b> | <b>Default Caution</b> | <b>Default Warning</b> | <b>Default Alarm</b> |
|---------------------------------------------------------------------------------------------------------------------------------------|---------------------------|------------------------|------------------------|----------------------|
| CO <sub>2</sub> <sup>1</sup>                                                                                                          | 10.0 %V/V<br>(5.0,50.0)   | Off                    | Off                    | Off                  |
| <sup>1</sup> <b>Not approved</b> for monitoring Carbon dioxide STEL (short-term exposure limit)<br>Contact factory for complete list. |                           |                        |                        |                      |

## **Standard range Nitrous Oxide (N<sub>2</sub>O) IR Sensor, 0-1%Vol , P/N 00-1431**

**Table 6. Target gas settings for the Standard-range N<sub>2</sub>O IR Sensor**

| <b>Target Gas Setting</b>                                                                                                            | <b>FS Range (Min,Max)</b> | <b>Default Caution</b> | <b>Default Warning</b> | <b>Default Alarm</b> |
|--------------------------------------------------------------------------------------------------------------------------------------|---------------------------|------------------------|------------------------|----------------------|
| N <sub>2</sub> O <sup>1</sup>                                                                                                        | 0.5 %V/V<br>(0.2,0.5)     | Off                    | Off                    | Off                  |
| <sup>1</sup> <b>Not approved</b> for monitoring Nitrous oxide STEL (short-term exposure limit)<br>Contact factory for complete list. |                           |                        |                        |                      |



## SPECIFICATIONS

**Table 7. Specifications**

|                            |                                                                                                                                                                                                                                                                                                                                                                                                                        |
|----------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Standard IR Sensor</b>  | <u>Standard LEL Hydrocarbon (HC) IR Sensor</u> , P/N 00-1375<br>For %LEL Methane, Ethane, Propane, n-Butane, and more (contact factory)                                                                                                                                                                                                                                                                                |
| <b>Optional IR Sensors</b> | <u>High-range Hydrocarbon (HHC) IR Sensor</u> , P/N 00-1376<br>Range 10-100 %VOL Propane, n-Butane, and LPG<br><u>Standard/low range Carbon Dioxide (CO2) IR Sensor</u> , P/N 00-1377<br>Range: 1-5 %VOL / Low range: 2000-5000 PPM<br><u>High-range Carbon Dioxide (HCO2) IR Sensor</u> , P/N 00-1378<br>Range: 5-50 %VOL<br><u>Standard range Nitrous Oxide (N2O) IR Sensor</u> , P/N 00-1431<br>Range: 0.2-1.0 %VOL |
| <b>Response Time</b>       | T90 < 30 seconds                                                                                                                                                                                                                                                                                                                                                                                                       |
| <b>Accuracy</b>            | Standard IR sensor: $\pm 2\%$ LEL (0.1%VOL) Methane<br>Optional sensors: $\pm 2\%$ of minimum range of target gas                                                                                                                                                                                                                                                                                                      |
| <b>Repeatability</b>       | Standard IR sensor: $\pm 2\%$ LEL (0.1%VOL) Methane<br>Optional sensors: $\pm 2\%$ of minimum range of target gas                                                                                                                                                                                                                                                                                                      |
| <b>Zero Drift</b>          | Standard IR sensor: $\pm 1\%$ LEL (0.05%VOL) Methane, per month<br>Optional sensors: $\pm 1\%$ of minimum range of target gas, per month                                                                                                                                                                                                                                                                               |
| <b>Span Drift</b>          | Standard IR sensor: $\pm 1\%$ LEL (0.05%VOL) Methane, per month<br>Optional sensors: $\pm 1\%$ of minimum range of target gas, per month                                                                                                                                                                                                                                                                               |
| <b>Humidity Range</b>      | 0 to 95 %RH non-condensing                                                                                                                                                                                                                                                                                                                                                                                             |
| <b>Analog Output</b>       | 4-20mA, 675 ohms max. at 24 VDC, current sourcing                                                                                                                                                                                                                                                                                                                                                                      |
| <b>AO Range</b>            | Standard IR sensor: 4mA is 0%LEL, 20mA is 100%LEL (programmable down to 50%LEL)<br>Optional sensors: 4mA is 0, 20mA is programmed gas range.                                                                                                                                                                                                                                                                           |
| <b>Serial Interface</b>    | HART® 1200 baud modem interface, registered DDL file, or Modbus ® 1200-600,14.4k,28.8k, RS232/RS485, or ASCII text output for printing data log                                                                                                                                                                                                                                                                        |
| <b>Power</b>               | 12 to 30 VDC (250 mA @ 24VDC maximum, 3-wire mode)                                                                                                                                                                                                                                                                                                                                                                     |
| <b>Alarm Relays</b>        | (3) SPST, contacts are rated at 5A@250 VAC, resistive load                                                                                                                                                                                                                                                                                                                                                             |
| <b>Relay Coils</b>         | Normally energized or de-energized, programmable                                                                                                                                                                                                                                                                                                                                                                       |
| <b>Enclosure</b>           | Explosion-proof, Class 1, Div. 1, Groups B, C, & D.                                                                                                                                                                                                                                                                                                                                                                    |
| <b>Controls</b>            | Non-intrusive (4 magnetic switches on front of transmitter)                                                                                                                                                                                                                                                                                                                                                            |
| <b>Operating Temp</b>      | -40° to +75° C                                                                                                                                                                                                                                                                                                                                                                                                         |
| <b>Weight</b>              | 4 Lbs. (1.8 Kg.)                                                                                                                                                                                                                                                                                                                                                                                                       |
| <b>Remote Sensor</b>       | Optional, 25ft. Max.                                                                                                                                                                                                                                                                                                                                                                                                   |



# INSTALLATION

## HAZARDOUS LOCATIONS

EXP-SNR transmitters are designed for use in hazardous locations rated Class 1, Division 1, Group B, C, or D. The transmitter should not be used in Group A environments (atmospheres containing Acetylene).

### When installing in a hazardous locations:

- 1) Connect the transmitter housing to earth ground.
- 2) Run wires in explosion-proof conduit and use an explosion-proof seal at the transmitter entry.
- 3) Seal the conduit entry both inside and outside of the transmitter housing to prevent condensation from leaking into the enclosure.
- 4) Follow national, state, and local electrical codes.

The transmitter can detect a variety of combustible gases and vapors. For gases that are heavier than air, such as Butane, sensors should be mounted near the floor. If the gas vapor has a density near that of air, locate the sensor about 5 feet above the floor in enclosed areas. Gas sensors mounted outdoors should be located near anticipated leak sources (valves, flanges, and compressors) and the location will depend on normal wind patterns and anticipated employee activity areas.

The following table lists common gases, along with their relative density (air = 1.00). Densities less than one indicate gases that are lighter than air while those with densities greater than one are heavier than air. Combustible vapors from most solvents, such as Benzene, n-Hexane, Methanol, Ethanol, and MEK, are heavier than air and will tend to accumulate near the floor in enclosed spaces with little air movement.

**Table 8. Gas densities relative to air.**

| Gas Name       | Density Relative to Air |
|----------------|-------------------------|
| Methane        | 0.55                    |
| Ethane         | 1.05                    |
| Propane        | 1.55                    |
| Butane         | 2.11                    |
| Carbon dioxide | 1.53                    |
| Nitrous oxide  | 1.53                    |

## **MECHANICAL MOUNTING**

Figure 6 shows the dimensions of the transmitter enclosure, and location and size of the electrical conduit opening. When used in a classified area, an explosion-proof seal should be installed as required by the local electrical code. If conduit is used, it must also be sealed internally at the housing entry to prevent condensation inside the conduit draining into the enclosure.


**Failure to seal the conduit entry or cable gland will result in water entering the enclosure causing damage to, or failure of, the transmitter electronics.**

The transmitter should be mounted with the sensor facing down. Transmitters are shipped with a protective plastic cap over the sensor that should be left in place during installation, and removed before placing the transmitter in service (leave the cap installed whenever painting around the transmitter).

|  |                                                              |  |
|--|--------------------------------------------------------------|--|
|  | <b>Remove protective cap from sensor prior to operation.</b> |  |
|--|--------------------------------------------------------------|--|

## **Supporting the Transmitter**

The transmitter should be secured to a wall or flat surface through two mounting holes in the enclosure, as shown in Figure 7. If proper conduit fasteners are used, the transmitter enclosure may be supported by conduit alone.

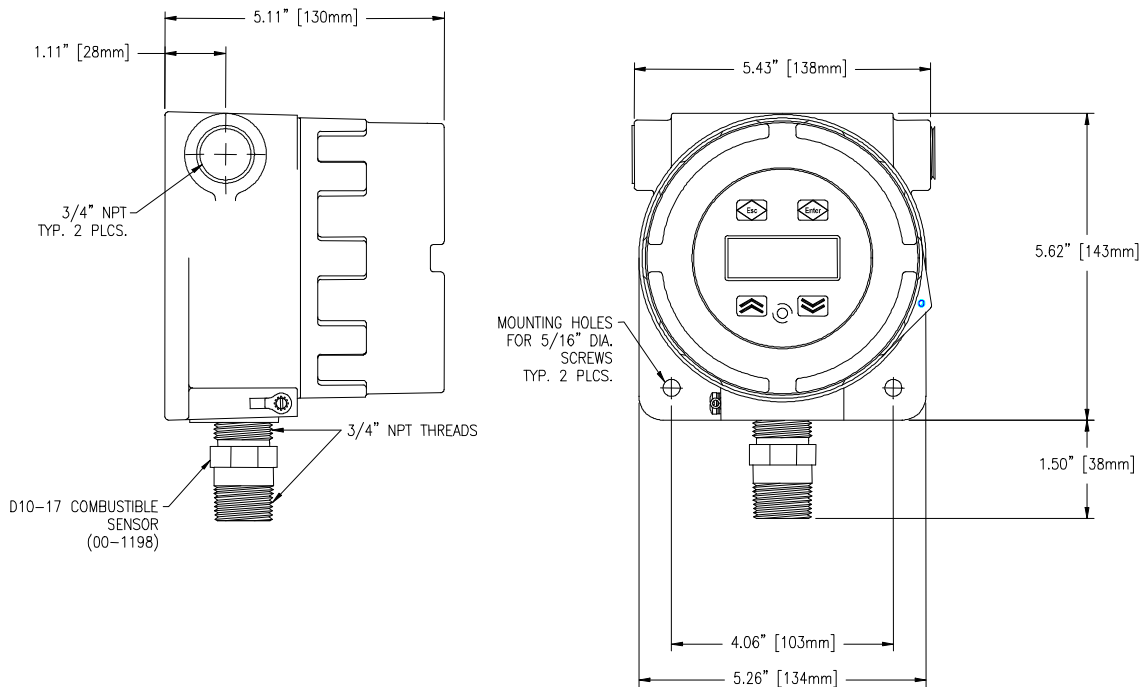

*Figure 7. Overall dimensions*

## **ELECTRICAL CONNECTIONS**

### **External Power Supply**

The transmitter requires a regulated DC supply, operating between 12 and 30 VDC. Transmitters ordered with relays will require a maximum current of 250mA, worst case (all relays energized). Power supplies for operating multiple units should be sized for twice the calculated load to allow for start-up (inrush) current.


### **The Stack**

The transmitter consists of three circuit boards, known collectively as the “stack”. From top to bottom, they are the, Display, CPU, and Power Supply. The top two boards, Display and CPU, are fastened together with metal standoffs, and plug into the Power Supply board, which is fastened to the lower housing with similar metal standoffs. Since most external wiring connections are made to terminals on the Power Supply board, it will be necessary to remove the top two boards.

**Please be aware of the hidden ribbon cable that connects the top two boards to the sensor. This cable is only long enough to permit the boards to come free from the housing.**

To remove the top boards, unscrew the transmitter housing cover and turn off the power switch, SW5, located at the 12 o’clock position on the CPU board. Grasp the outer edge of the metal faceplate covering the Display board and gently rock it side to side, while pulling it up, and away from the housing. Once the top boards come free, lift them out and disconnect the sensor ribbon cable (note: this connector is keyed for ease of reconnecting later).

**Set switch SW5 to OFF before removing the upper board stack from the transmitter. Since SW5 does not disconnect power at the terminals of the Power Supply Board, declassify hazardous areas prior to opening the transmitter housing.**

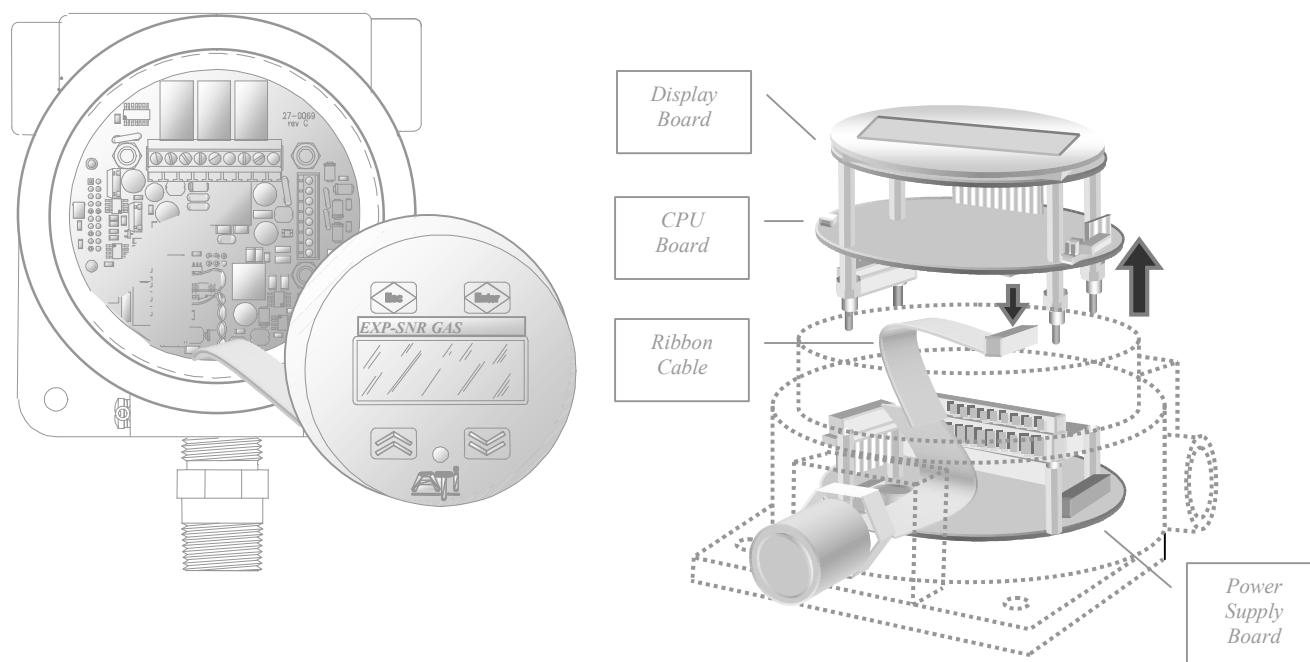

**Figure 8. Accessing Electrical Connections**

### **Power Supply Board**

Electrical connections are made to terminal blocks TB1 and TB2. The 4-20mA current loop, optional digital communications, and remote alarm reset, are connected at TB1. Connections to the three optional relays are made at TB2. It is recommended to power the transmitter, and all controls and indicators, from separate, uninterruptable supplies.

Note: This version of the transmitter cannot operate on loop power alone.

The transmitter requires primary power in the range of 12 to 30 VDC applied to pins 7 and 8 on TB1. Current loop operation requires power in the same range on pin 5 (mA+), from which the transmitter sources a positive, 4-20mA output on pin 6 (mA-).

#### ***IMPORTANT***

The loop supply voltage on pin 5 must not exceed the primary supply voltage on pin 8.

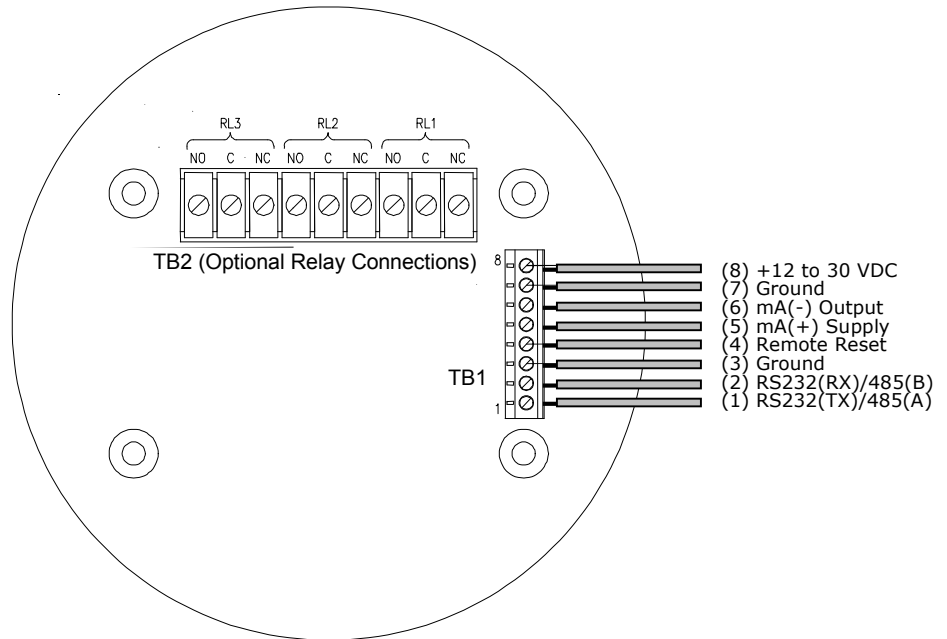


Figure 9. Power supply board connections.

In 3-wire mode, the transmitter requires a maximum of 250 mA, with all relays active. Power supplies operating multiple units should be sized for twice the calculated current requirement to allow for inrush current during startup.

The housing has limited space for wire. Use the smallest gauge wire available that is compatible with electrical code and current requirements. When powering a group of transmitters in 3-wire mode from the same power supply, 12 AWG wire is recommended for long runs, with smaller (higher gauge) wire drops to each transmitter.

Internal relays are best used as pilot relays if heavy load switching is desired. Use suitable arc suppression devices across loads switched through internal relays.

The transmitter housing may be grounded through explosion proof conduit. In the absence of such conduit, use a suitable grounding strap to bond the transmitter's housing to earth ground.

**Always follow wiring practices governed by local, state, and national electrical codes.**

**Relay Contacts**

Note: the behavior described below is determined by the default relay settings, which may be reprogrammed through the operator or communication interface.

By default, RL1 is de-energized until the gas concentration reaches the Warning level, and is then energized until the alarm is cleared, or power fails. Likewise, RL2 is de-energized until the gas concentration reaches the Alarm level, and is then energized until the alarm is cleared, or power fails. In contrast, RL3 is energized until a Fault condition is detected, or power fails, and is then de-energized until the condition is cleared.

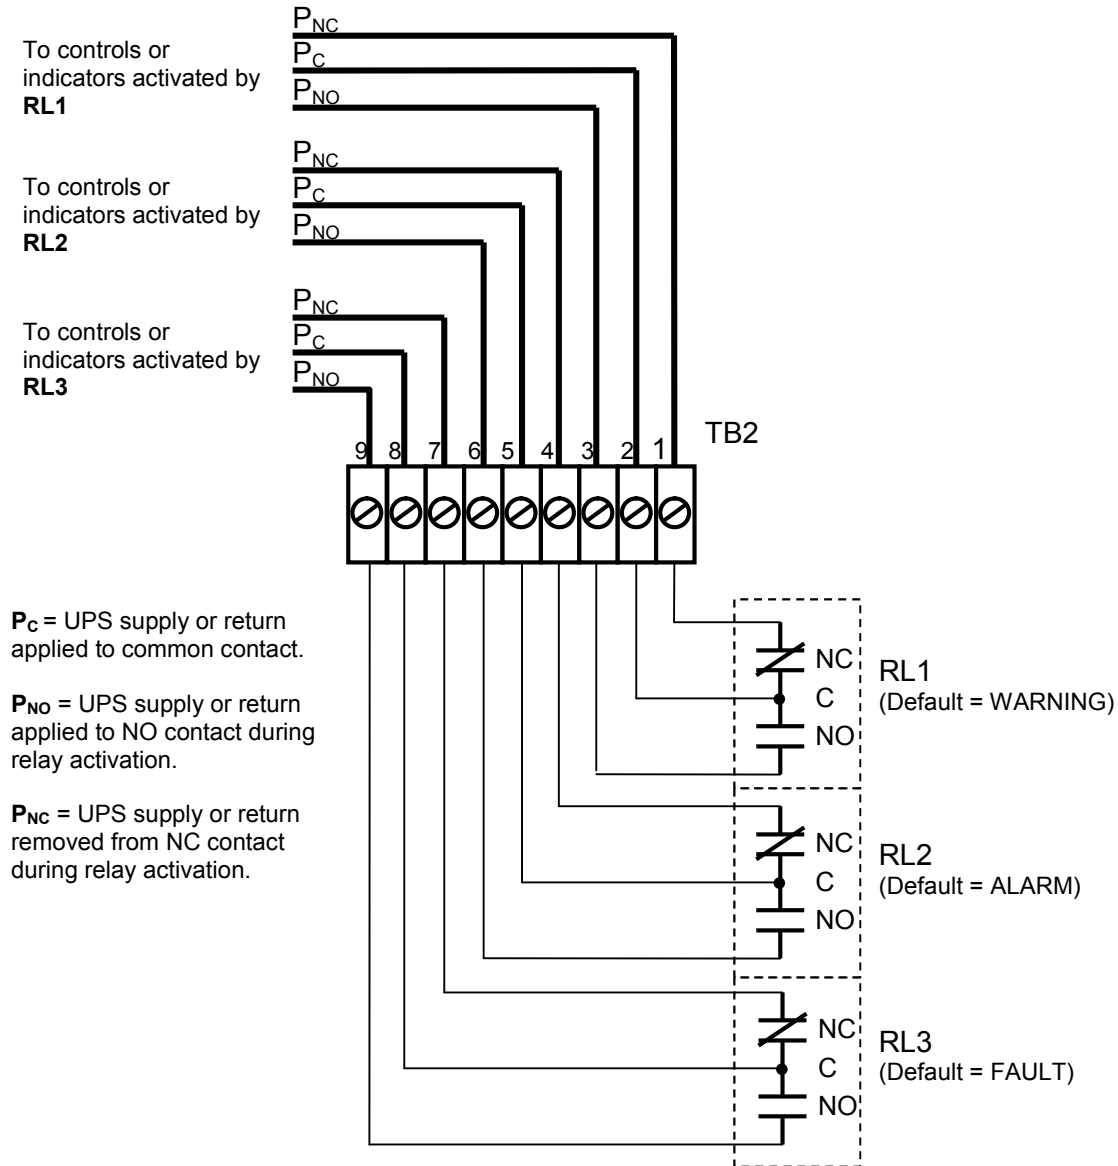



Figure 10 Relay Contacts

**Series EXP-SNR Gas Transmitter with IR Sensor**

**Wiring Examples**

**A17/B14, 3-Wire Mode**

A single A17 may be used to power one EXP-SNR transmitter in 3-wire mode and one B14 receiver (see B14 Monitor O&M Manual).

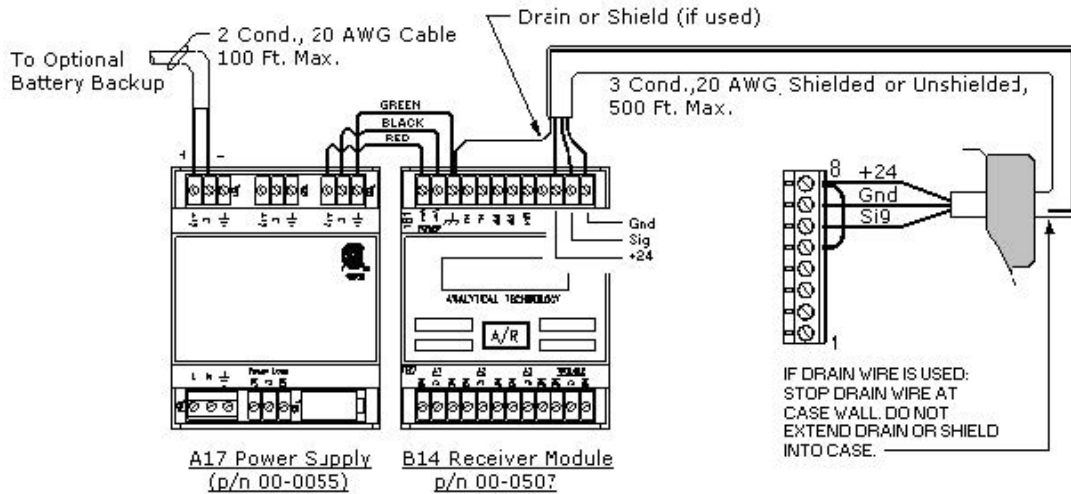


(see B14 Monitor O&M Manual)

*Figure 11. A17/B14 Example*

**Power Without 4-20mA Signaling**

Power without 4-20mA signaling is not common practice, except when signaling digitally over HART multidrop and Modbus connections. There are several examples of those in the pages that follow.

When 4-20mA signaling is not used, the transmitter may be powered solely from TB1-7 and 8, which are connected directly to the supply (note 1). Multiple transmitters may be powered this way, as shown. Size each power supply according to the number of transmitters, the current demand of each (see specifications), and the wire resistance. The wire resistance must not be allowed to drop the primary supply voltage below 10V at the primary supply terminals of any transmitter. Hint: If possible, use 12-14 AWG wire on primary supply connections, keep the number of transmitters low, and verify the voltage on the on the transmitter furthest from the supply.

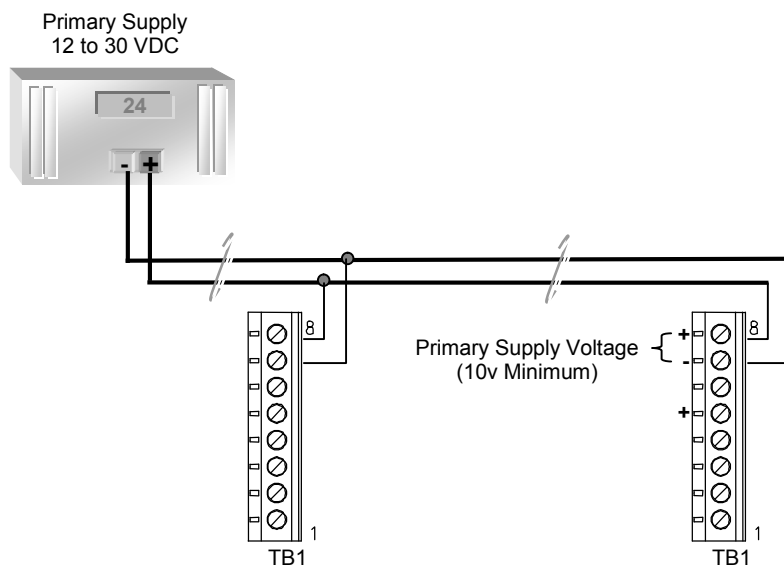

*Figure 12. Power Without 4-20mA Signaling Example*

**Notes**

1. Power without 4-20mA signaling is not common practice, except for HART multidrop or Modbus connections that use digital signaling (not shown), providing a local alarm, or both. Power shown above is sufficient for Modbus connections, relays, and LCD backlight operation.

### 4-20mA Signaling, Single Supply, 3-Wire Mode

Multichannel Current Loop Receiver with Integral 24V Supply

(Channels are typically not isolated from supply)

0.0

+24

+

-

Gn

Sig

Primary Supply Voltage (10v Minimum)

8

1

TB1


Rev. K (7/15)

**4-20mA Signaling, Dual Supply, 4-Wire Mode**

To reduce the power requirement of a single current loop supply, the transmitter may be powered from both a primary and loop supply, providing the following conditions are met.

1. Supply grounds are directly connected to minimize ground loops, and,
2. The Primary Supply Voltage must not drop below the Loop Supply Voltage, as measured at instrument terminals.

Size each power supply according to the number of transmitters, the current demand of each (see specifications), and the wire resistance. The wire resistance must not be allowed to drop the Primary Supply Voltage below the Loop Supply Voltage, as measured at the terminals of any transmitter. Hint: select a Primary Supply with a higher voltage output than the Loop Supply, and use 12-14 AWG wire, if possible. Keep the number of transmitters supplied by the Primary Supply low, and verify the voltages at the terminals of the transmitter furthest from the Primary Supply.

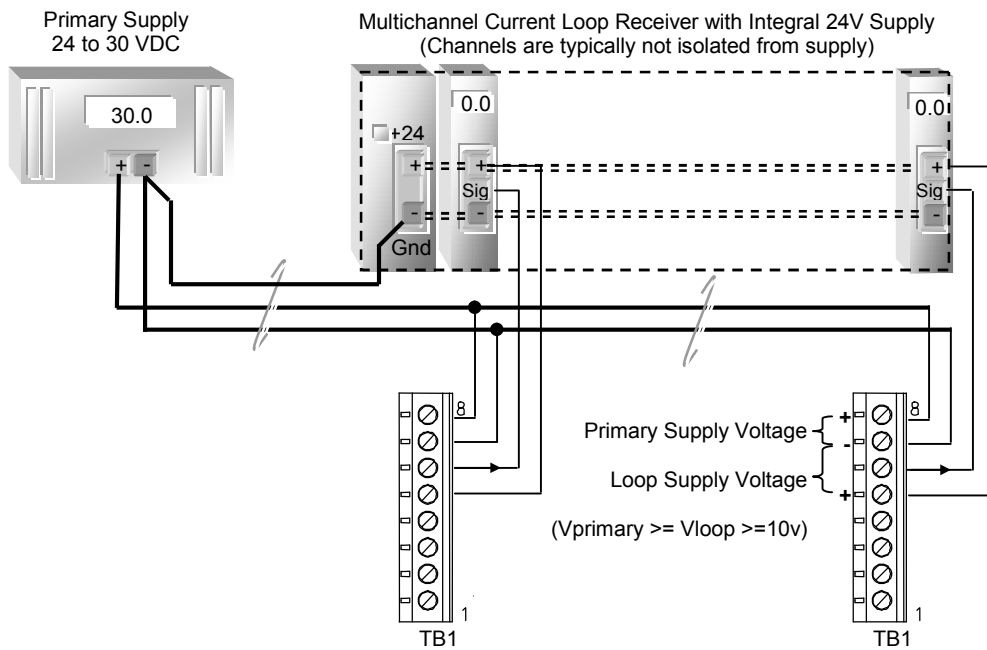

**IMPORTANT**

Primary Supply Voltage must not drop below Loop Supply Voltage at terminals of any transmitter.


Hint: Use 12 AWG wire on Primary supply connections to minimize voltage drops.

- 1 Select a Primary Supply with a higher voltage output, and,
- 2 Connect supply commons to minimize ground loops and voltage drops that might reduce the Primary Supply Voltage below the Loop Supply Voltage, at transmitter.

*Figure 14. 4-20mA Signaling, Dual Supply, 4-Wire Example*

**HART Transmitter, Point-to-Point, 3-Wire (Active Source)**


The HART “Point-to-Point” connection permits the transmitter to communicate digitally, while retaining the functionality of its 4-20mA current loop. Setting the transmitter’s polling address to 0 permits the current loop to function normally. According to HART specifications, the current loop must be terminated with a load resistor between 230 and 1100 ohms; however, transmitter specifications restrict the maximum analog output resistance to a lower value (see Specifications). The term, “active source”, refers to a transmitter that is not loop powered, and sources current from power applied to it on separate terminals. Size the power supply according to the number of transmitters, the current demand of each transmitter (see specifications), and wire resistance. Wire resistance must not be allowed to drop the Primary Supply Voltage below 10V at the terminals of any transmitter. Hint: use at least 14 AWG wire on supply connections (shown in bold).

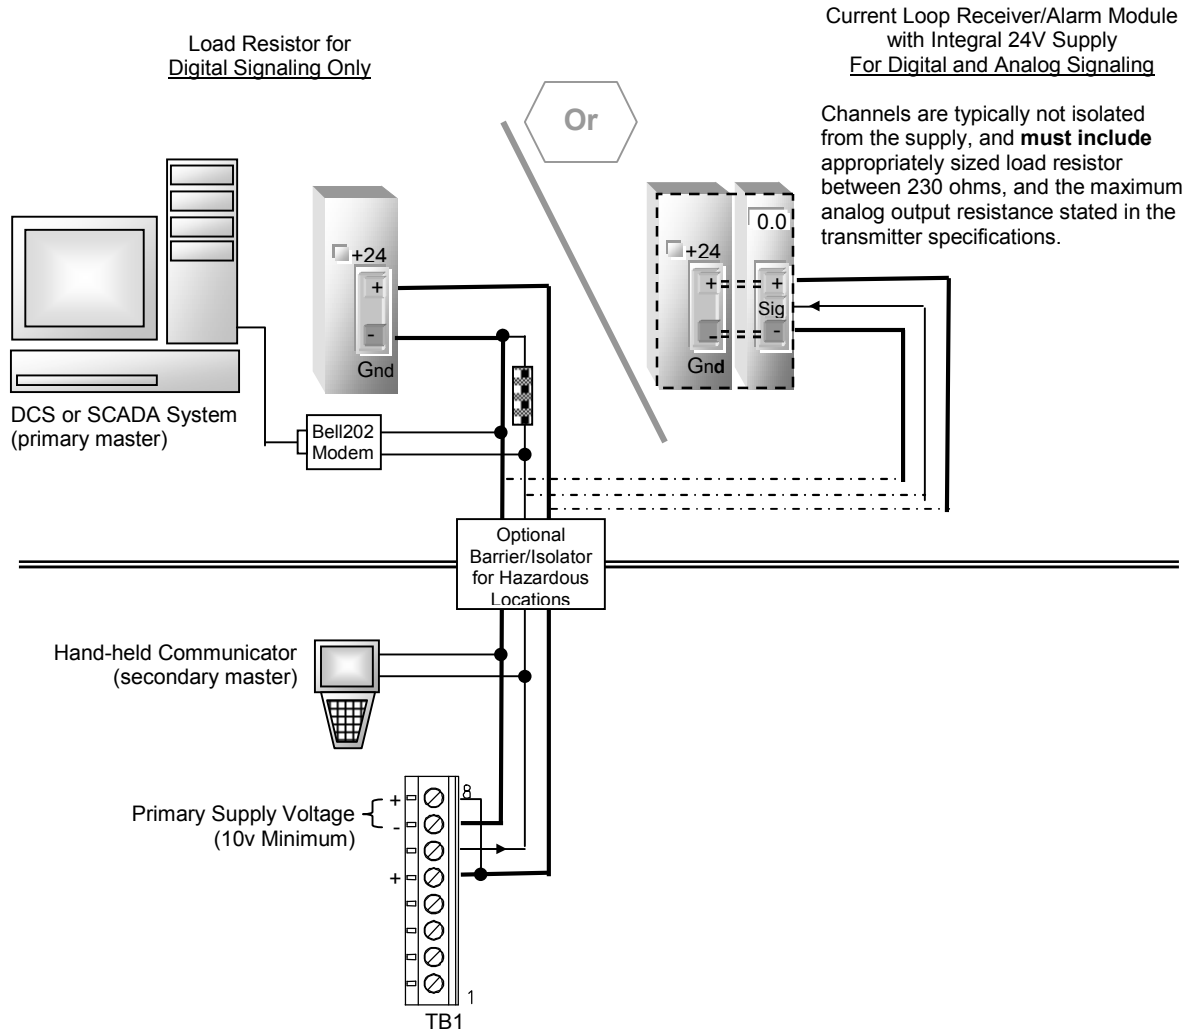

**Figure 15. HART Transmitter, Point-to-Point, 3-Wire Example**

**HART Transmitter, Multi-drop, 3-Wire (Active Source)**

The HART “Multi-drop” connection permits up to 15 transmitters to communicate digitally on the same bus, but at the cost of analog current signaling. Setting the transmitter’s polling address from 1 to 15 fixes the current loop output at 4mA. According to HART specifications, the current loop must be terminated with a load resistor between 230 and 1100 ohms; however, transmitter specifications restrict the maximum analog output resistance to a lower value (see Specifications). The term, “active source”, refers to a transmitter that is not loop powered, and sources current from power applied to it on separate terminals. Size the power supply according to the number of transmitters, the current demand of each transmitter (see specifications), and wire resistance. Wire resistance must not be allowed to drop the Primary Supply Voltage below 10V at the terminals of any transmitter. Hint: use at least 14 AWG wire on supply connections (shown in bold).

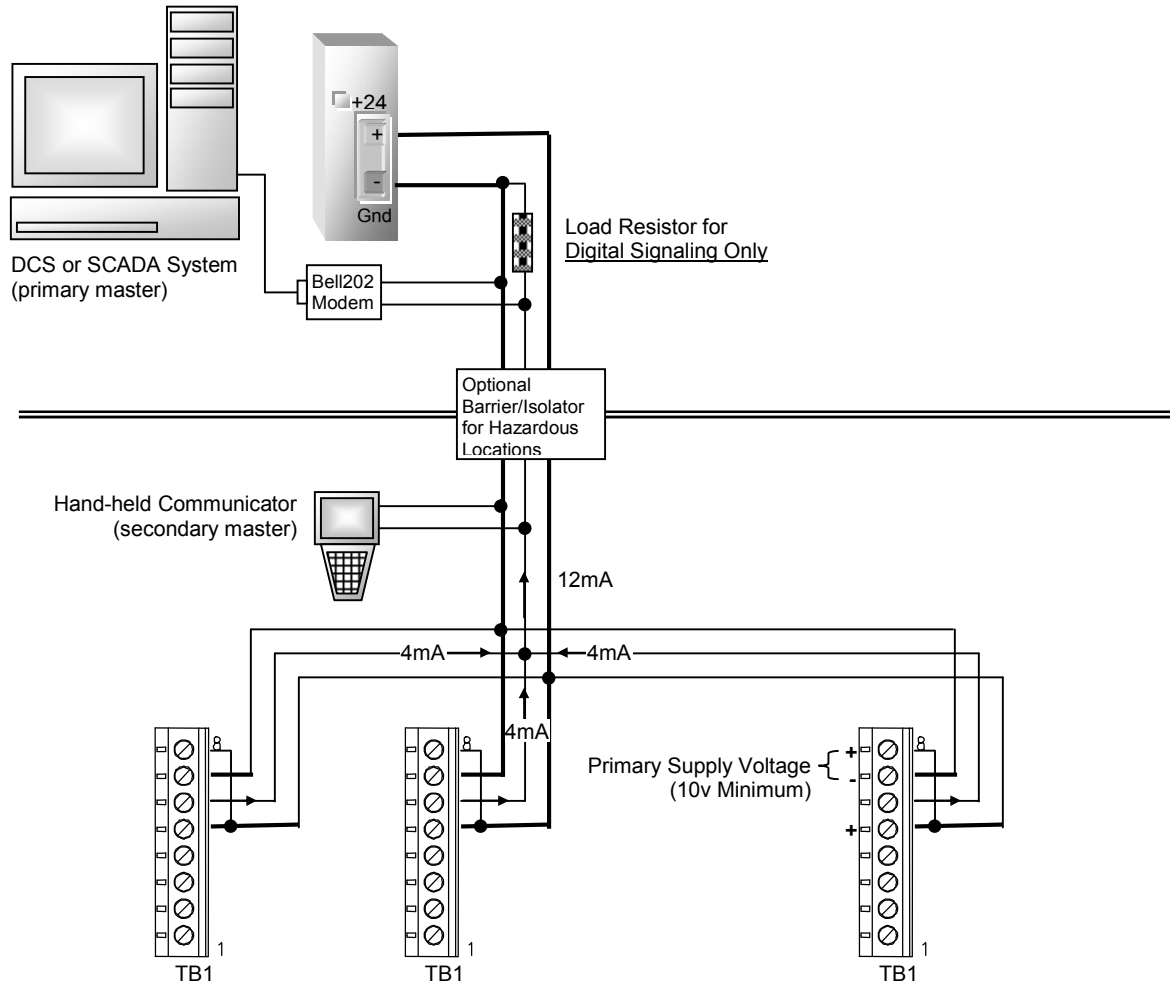


*Figure 16. HART Transmitter, Multi-drop, 3-Wire Example*



**RS232 Modbus, PC Capture, or Printer**

RS232 operation requires the transmitter to be wired in 3- or 4- wire mode. In addition, the RS232 COM jumper must be installed at JP4 on the CPU board. The RS232 connection may be used for a Modbus connection, capturing the data log output using a PC, or printing the data log output to an Epson compatible printer. Refer to the **Modbus Interface Manual** for details on Modbus connections and implementation, and to Appendix A on page 70 for details on outputting data log reports.

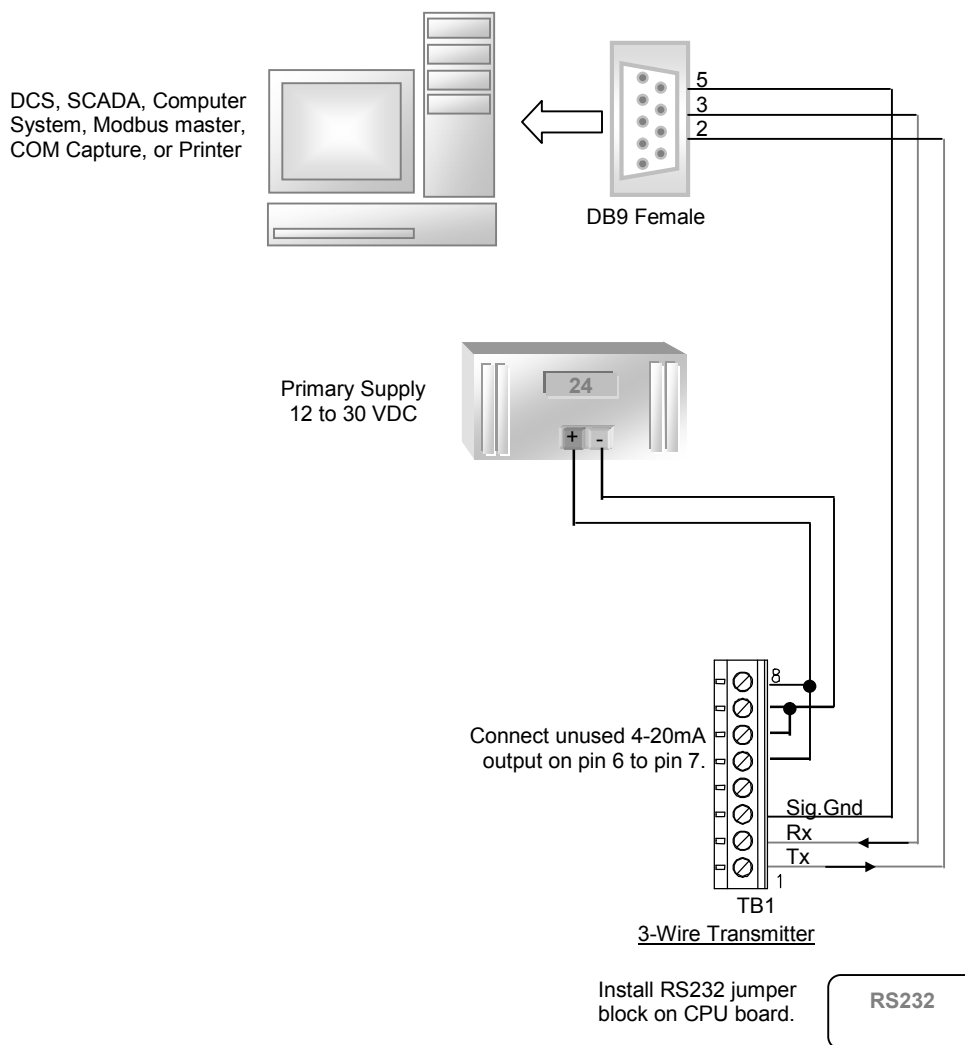


*Figure 18. RS232 Modbus, PC Capture, Printer Example*

**Series EXP-SNR Gas Transmitter with IR Sensor**

**Remote Sensor Wiring**

The remote sensor option allows separation of the sensor and transmitter by up to 25 feet. The sensor is threaded into a junction box, and connected to the transmitter using a supplied cable, which may be shortened, if necessary. The figure below shows the wiring connections at each end.

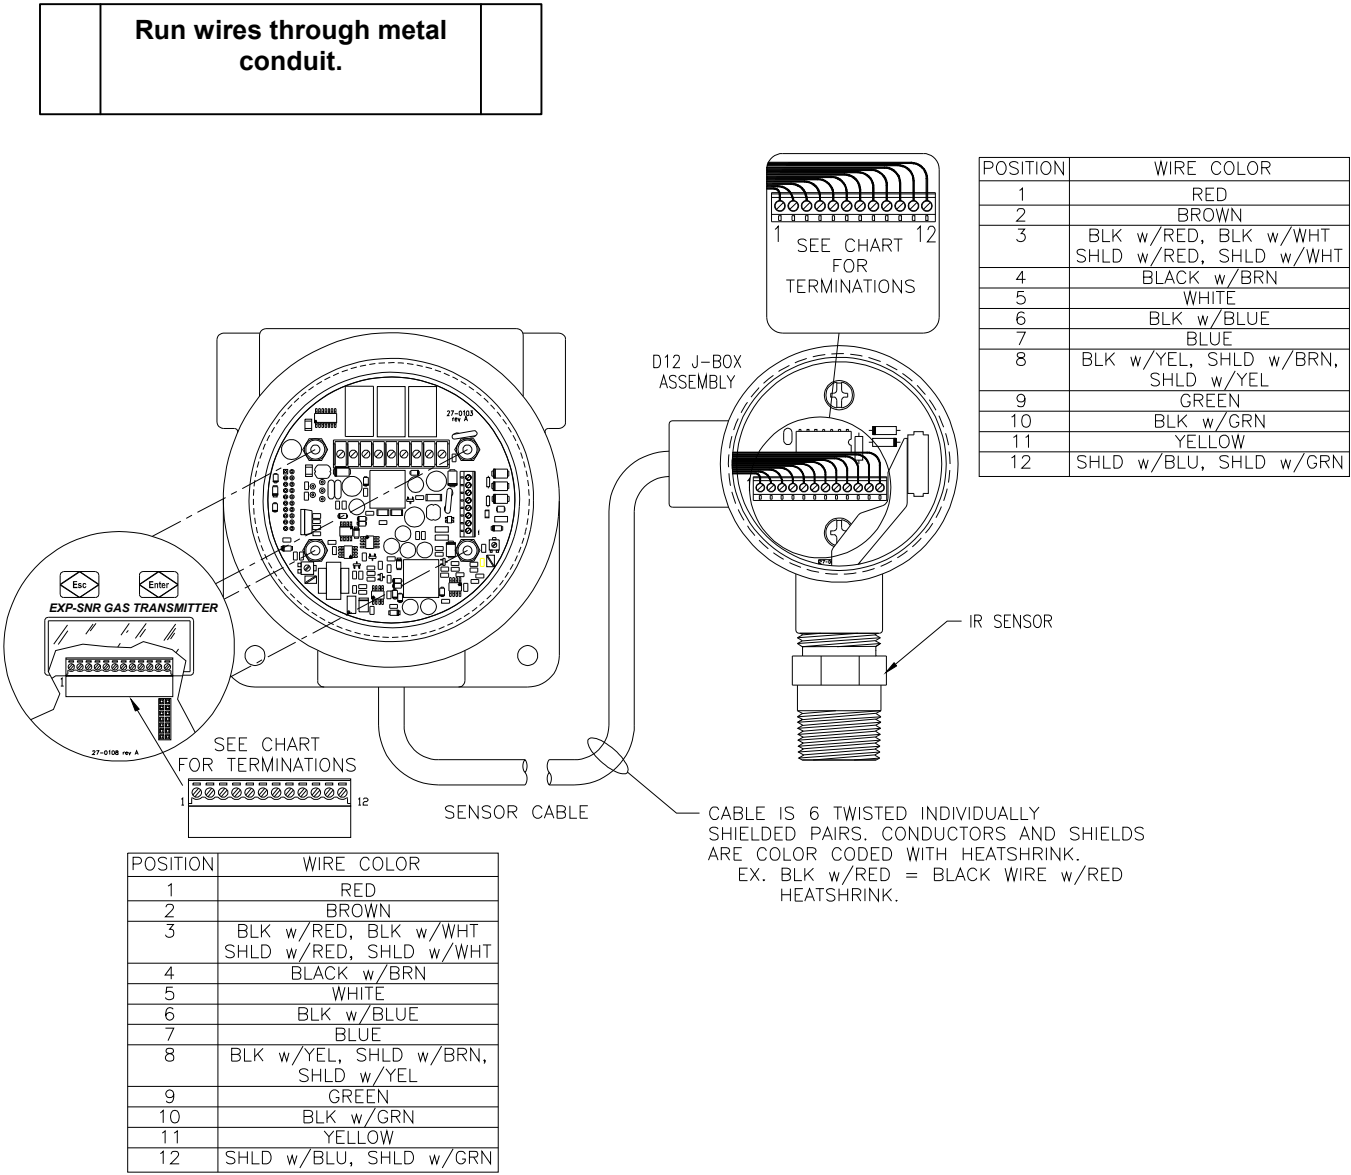


*Figure 19. Remote Sensor Option wiring*

## CPU Board Configuration

If required, install a communications jumper plug on JP4 based on the protocol and interface options shown in Table 9. If equipped with relays, install a jumper on JP1, pins 3-4.

**Table 9. Communication option jumpers**

| <b>Protocol</b> | <b>Interface</b> | <b>Jumper Plug Label</b> | <b>Comments</b>                                                                                                                                                                                                                                                                                        |
|-----------------|------------------|--------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| HART            | Bell 202         | None Required            | Okay to install any.                                                                                                                                                                                                                                                                                   |
| Modbus          | RS232            | "RS232"                  | Use to connect one transmitter to a master device in a "point-to-point" configuration. See "EXP-SNR Modbus Manual" for details.                                                                                                                                                                        |
| Modbus          | RS485            | "RS485"                  | Use to connect up to 4 transmitters to a master device in a "multi-drop" configuration. Each transmitter connection biases and terminates the transmission line, as shown below. See "EXP-SNR Modbus Manual" for details.                                                                              |
| Modbus          | RS485            | "RS485 Unterminated"     | Use to connect more than 4 transmitters to a master device in a "multi-drop" configuration. Transmitters are connected without adding bias or termination. Install one (terminating) "RS485" jumper plug on transmitter at furthest end of transmission line. See "EXP-SNR Modbus Manual" for details. |
| ASCII           | RS232            | "RS232"                  | Use to connect one transmitter to a printer, or system terminal (see Datalogging section).                                                                                                                                                                                                             |

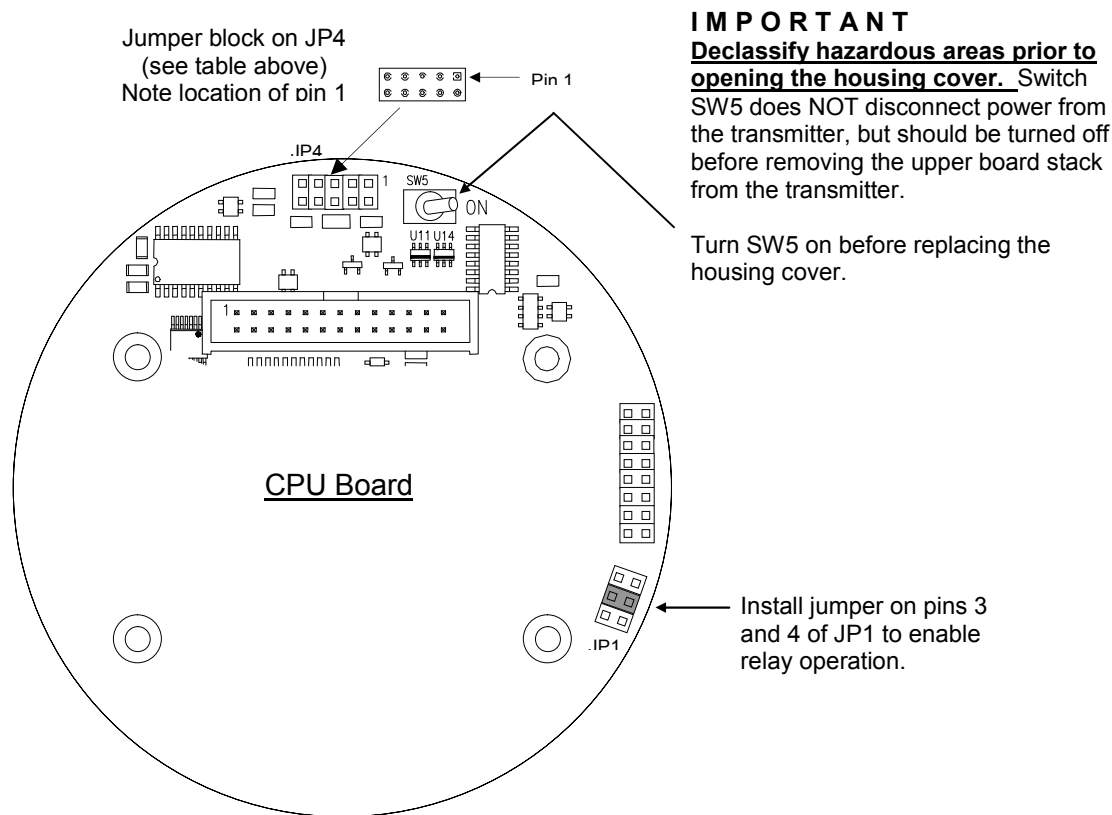

*Figure 20. CPU Board configuration*


**Series EXP-SNR Gas Transmitter with IR Sensor**

## OPERATION



### Interface Panel

The EXP-SNR operator interface is non-intrusive, so you do not have to remove the housing cover to view the display, configure the transmitter, or calibrate the sensor. It features a back lighted\*, 96x32 dot LCD display, and four “keys”. The keys are implemented as four magnetic switches, each centered below a graphic icon, and activated when a magnet is held approximately 1/4” above the icon. The transmitter is provided with a powerful, magnetic-screwdriver, designed specifically for activating the switches through the housing’s thick, glass window. Throughout this manual, activating keys in this manner is referred to as, “touching” the keys, even though it is not necessary to make physical contact.

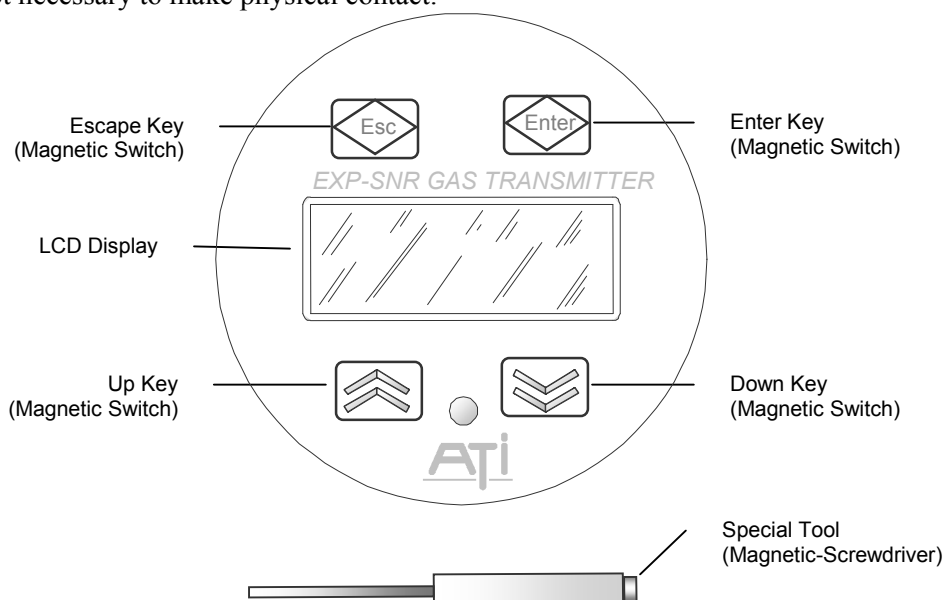

*Figure 21. Operatore Interface Panel*

The operator interface is organized into pages that consist mostly of text objects representing readings, indicators, variables, functions, and links to other pages. Navigating the pages of objects is simplified through the use of a “point-and-click” interface, using an arrow cursor that may be moved from one object to the next by “touching” the up or down key. While the cursor is “pointing” at an object, touching the magnet to the Enter key is said to “select” the object, and the action performed depends on the type of object. If the object is a function, the Enter key executes the function. If a variable is selected for editing, the Up and Down keys change its value, and the Enter key saves it. Touching the Esc key aborts the edit and restores the previous value. If not executing a function, or editing a variable, touching the Esc key returns to the previous page.

(\* back-lighting available in 3- or 4-wire mode, only)

## Startup Review Sequence

When the transmitter starts, the display cycles through a series of pages to review the configuration of the transmitter, sensor, and generator. Alarms are inhibited, and the output of the transmitter is held at 4.0 mA. This state is maintained for 5 minutes to provide time for the sensor readings to stabilize.

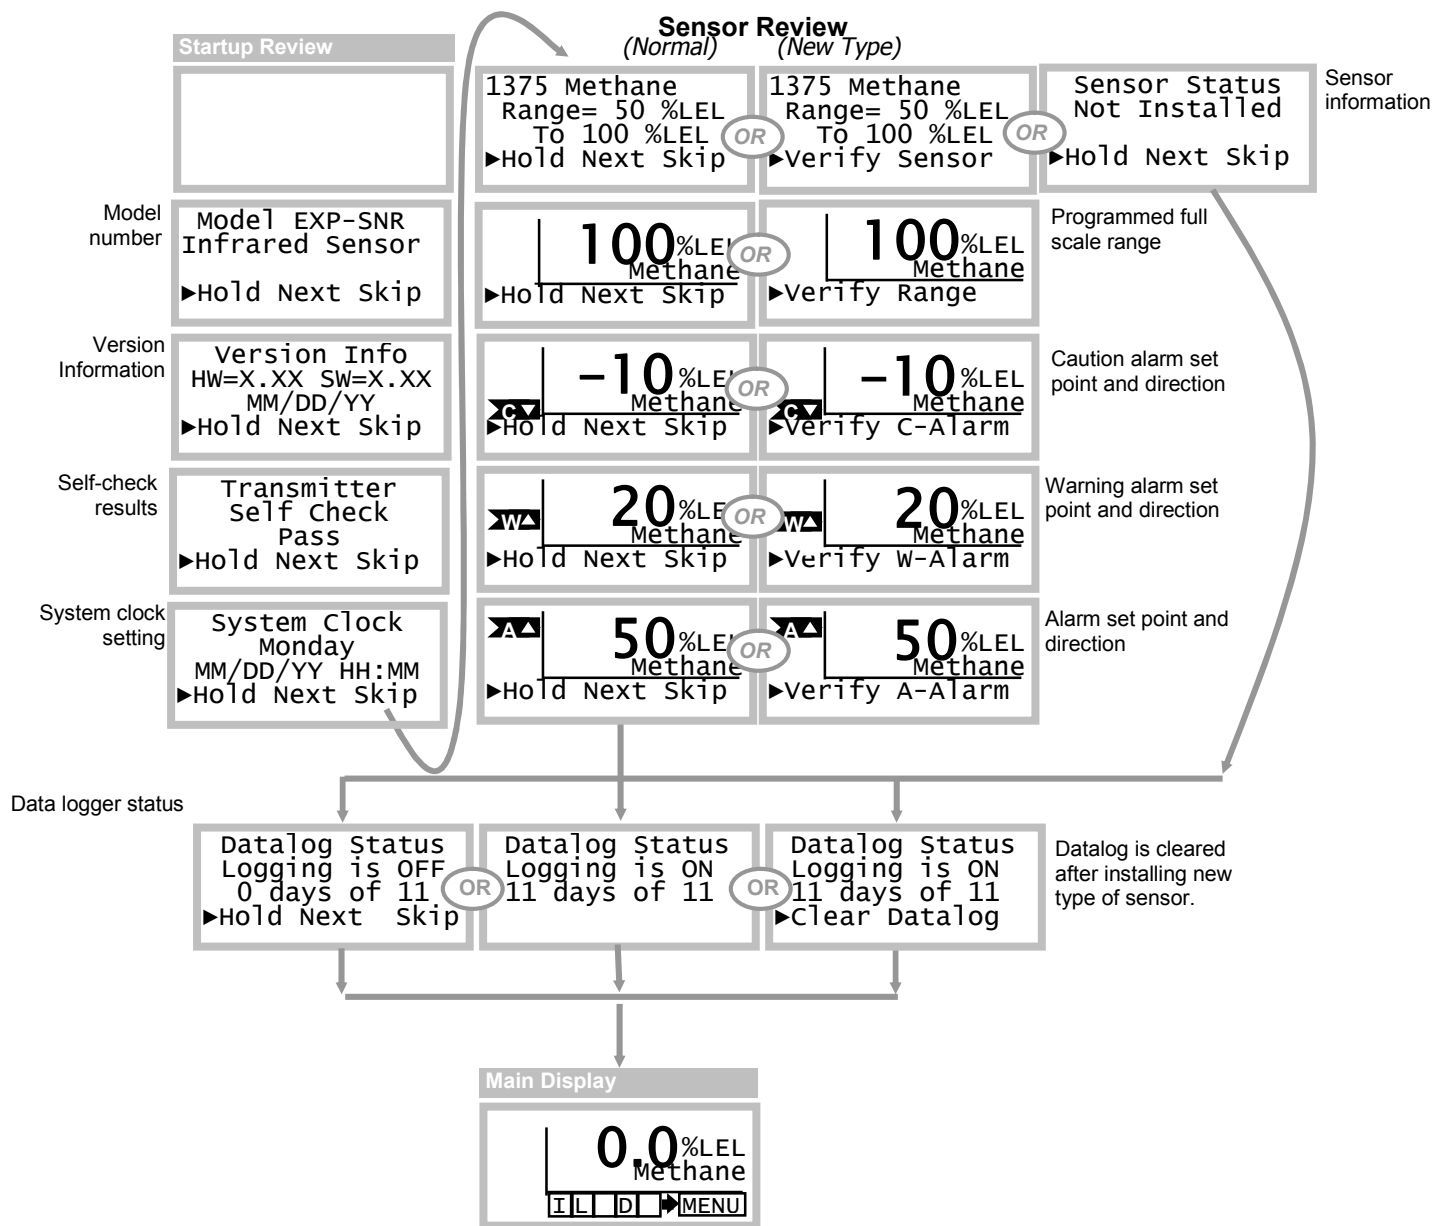


Figure 22. Startup review sequence

## Main Display Page

The Main Display Page shows the name and concentration of the target gas, and units of measurement (%LEL, %V/V, PPM, etc). Indicators on the left and below show alarm and operating status.


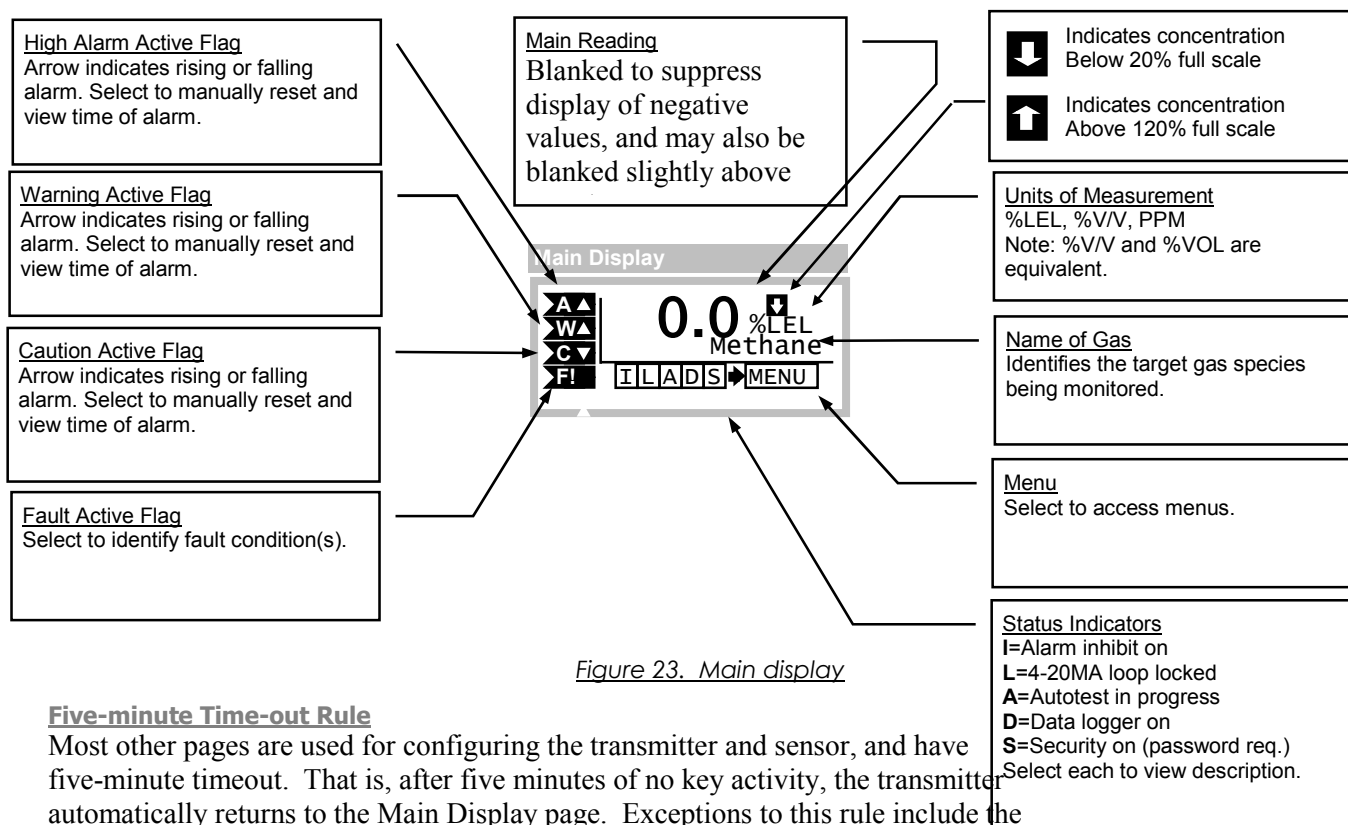


Figure 23. Main display

## Five-minute Time-out Rule

Most other pages are used for configuring the transmitter and sensor, and have five-minute timeout. That is, after five minutes of no key activity, the transmitter automatically returns to the Main Display page. Exceptions to this rule include the zero and span calibration pages.

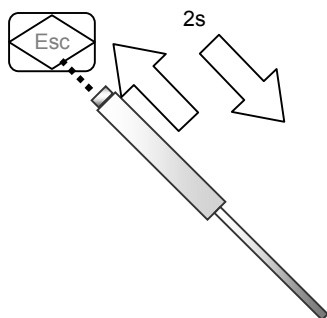


## Esc Key Operation - Main Display Only

Holding the magnet over the ESC key for 2 seconds, then removing, toggles alarm inhibit mode on and off. If the alarm inhibit mode was off, it is turned on for 15 minutes (default value). If alarm inhibit was on, it is turned off immediately. Alarm inhibit mode is on when the "I" status indicator is visible.


## Fault Indication

Faults are indicated on the Main Display Page as shown below.

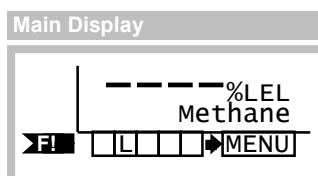

### **Main Reading**

The main reading represents the gas concentration value and appears on the Main Display, along with the sensor name, and units of concentration. It is reported on the 4-20mA output<sup>1</sup>, and is the PV (Primary Variable) reported on the optional HART™ interface. It also appears at register 40043




(EXP-SNR\_SYS\_CONCBL) on the optional Modbus interface.

By default, the main reading is blanked to suppress the display of negative values. That is, the reading is reported as zero if the concentration should dip below zero, which can occur over time as a result of sensor aging. If the concentration falls to – 20% of the full-scale range, a fault alarm is generated. Blanking is typically extended slightly above zero, as a means of stabilizing the main reading in the presence of excessive external noise, or other environmental factors (see Sensor Setup Pages).

During zero and span calibration, the “un-blanked” gas concentration value is displayed, primarily to assess the amount of positive or negative drift. The “un-blanked” reading is also available on the Modbus interface (request “EXP-SNR Transmitter Modbus Interface Manual”, for more information).

### **Menu Page**

The MENU page provides direct access to the zero and span calibration functions, and to the data log graphics page. It also provides access to the setup page for configuring the transmitter. To access it from the Main Display page, touch the magnet to the up or down key until the cursor is pointing to the **MENU** icon, then touch the Enter key.

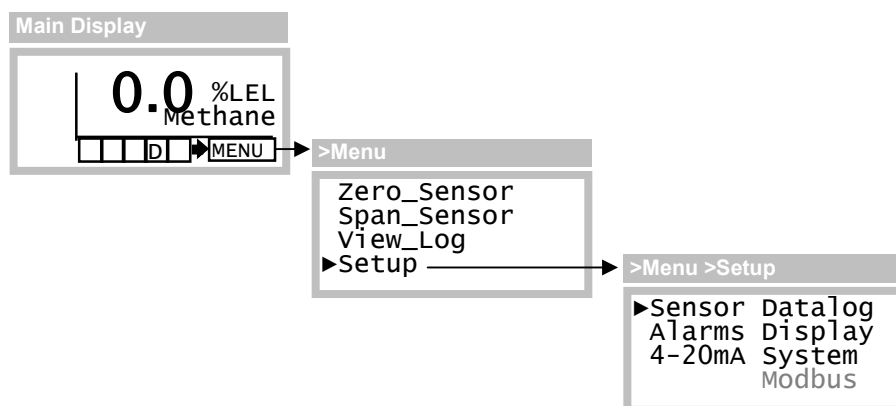

*Figure 24. Menu and Setup pages.*

### **Setup Page**

The Setup page lists the pages used to configure the operation of the transmitter. The contents of each of these pages are included as part of the description of each function, in the sections that follow.

<sup>1</sup> The 4-20mA may not correspond to the reading when the “L” status indicator is visible on the Main Display, or when the output is in a physical limit.

### **Variable Editing**

When a variable is selected, the edit cursor appears. The shape of the cursor symbolizes the up-down scroll nature of the value being edited. To provide feedback about which key is being activated, the cursor changes to a solid up-arrow when the magnet is touching the Up key, and to a solid down-arrow when the magnet is touching the Down key. When the variable has been adjusted to the desired value, touching the magnet to the Enter key changes the cursor to an hourglass shape while the program is saving the new value (recalculating associated variables and updating non-volatile memories). Touching the magnet to the Esc key discards the edited value and restores the original value.

### **Cursors**



- |                                                                                                      |                                                                                                             |                                                                                                                                                                                                        |                                                                              |
|------------------------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------------|
| <p>1. On entry, the select cursor points to the first variable for editing.</p>                      | <p>&gt;Menu &gt;Setup &gt;4-20mA</p> <p>▶Autotst_mA= 4.0<br/>Inhibit_mA= 4.0<br/>Fault_mA= 3.6<br/>More</p> | <p>&gt;Menu &gt;Setup &gt;4-20mA</p> <p>Autotst_mA= 4.0<br/>Inhibit_mA= 4.0<br/>▶Fault_mAX 3.7<br/>More</p>                                                                                            | <p>6. Touch the magnet to the ENTER key to save the edited value, or...</p>  |
| <p>2. Touch the magnet to the UP or DOWN key to move the cursor to the desired item.</p>             | <p>&gt;Menu &gt;Setup &gt;4-20mA</p> <p>Autotst_mA= 4.0<br/>Inhibit_mA= 4.0<br/>▶Fault_mA= 3.6<br/>More</p> | <p>&gt;Menu &gt;Setup &gt;4-20mA</p> <p>Autotst_mA= 4.0<br/>Inhibit_mA= 4.0<br/>▶Fault_mA= 3.6<br/>More</p>                                                                                            | <p>7. Touch the magnet to the ESC key to cancel the edit without saving.</p> |
| <p>3. Touch the magnet to the ENTER key to edit the item, the edit cursor appears.</p>               | <p>&gt;Menu &gt;Setup &gt;4-20mA</p> <p>Autotst_mA= 4.0<br/>Inhibit_mA= 4.0<br/>▶Fault_mAX 3.6<br/>More</p> | <div style="border: 1px solid gray; padding: 10px; display: inline-block;"> <p>Main Display</p> <p style="font-size: 2em; font-weight: bold;">0.0</p> <p>%LEL Methane</p> <p>□ □ □ □ □ MENU</p> </div> |                                                                              |
| <p>4. Touch the magnet to the UP key to increment the value, and the increment cursor appears.</p>   | <p>&gt;Menu &gt;Setup &gt;4-20mA</p> <p>Autotst_mA= 4.0<br/>Inhibit_mA= 4.1<br/>▶Fault_mA▲ 3.8<br/>More</p> |                                                                                                                                                                                                        |                                                                              |
| <p>5. Touch the magnet to the DOWN key to decrement the value, and the decrement cursor appears.</p> | <p>&gt;Menu &gt;Setup &gt;4-20mA</p> <p>Autotst_mA= 4.0<br/>Inhibit_mA= 3.9<br/>▶Fault_mA▼ 3.7<br/>More</p> |                                                                                                                                                                                                        |                                                                              |

*Figure 25. Variable editing*


<sup>2</sup> Range is restricted between 100 and 50 when equipped with the HC sensor.

## Sensors

The operator interface includes several pages for configuring the sensor, and accessing its calibration history.

### Sensor Setup Pages

#### Sensor Target Gas, Range, Units, and LEL Variables

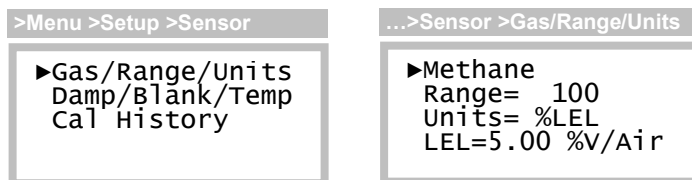


*Figure 26. Sensor setup and Gas/Range/Units pages*

**Table 10. Sensor target gas, range, units, and LEL variables**


| Variables            | Description                                                                                                                                                                                                                                                                                                    |
|----------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Gas Name<br>(line 1) | The name of the target gas appears on line 1. During edit, the setting may be scrolled up and down to select a different gas. Only gasses that have been span calibrated at the factory will appear.                                                                                                           |
| Range                | The Range variable sets the full-scale value of the transmitter, which corresponds to the 20mA output value. Changing the range value also changes the Blanking value, which is computed as a fraction of the range. If data logging is enabled, a warning is displayed when the value is changed (see below). |
| Units                | The Units variable affects all concentration readings appearing at the transmitter, and over the Modbus and HART interface. Selections are dependent on the target gas selection, and In some cases, the setting is restricted to only one selection.                                                          |
| LEL                  | The LEL variable is read only and appears for gasses that may be displayed in units of %LEL (explosive gasses). The displayed value is the volumetric mixture ratio corresponding to 100 %LEL, and is provided to overcome any ambiguity in the %LEL reading.                                                  |

The data-logger records readings as a fraction of the sensor range. If data logging is turned on (indicated by “D” status indicator on the Main Display), changing the Range variable causes a warning message to appear prior to saving the value. Select “Save” to save the new Range variable, or “Abort” to leave it unchanged.

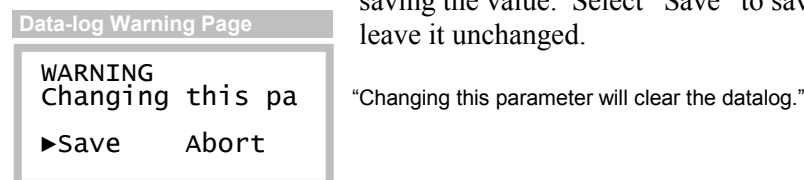

*Figure 27. Data-log warning page*

**Sensor Damping, Blanking, and Temperature Variables**

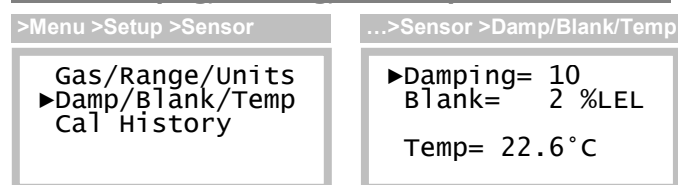


*Figure 28. Sensor setup and Damp/Blank/Temp setup page*

**Table 11. Sensor damping, blanking, and temperature variables.**

| Variables | Description                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                              |
|-----------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Damping   | The Damping variable allows minor adjustment of the transmitter's auto-damping feature, used to stabilize readings. It is a unit-less value from 1 to 100, where a value of 1 corresponds to a T90 <sup>3</sup> response of approximately 20s, and 100 is a T90 of approximately 30s. The default value is 10, resulting in a T90 response of approximately 21s.                                                                                                                                                                                         |
| Blank     | <p>The Blank (blanking) variable is used to force the main reading to zero, whenever the gas concentration is below the programmed value. Blanking is normally limited from 0 to 10 % of Range, but varies by target gas selection. Note that the transmitter always performs negative blanking, even when Blank is set to 0.</p> <p>The Blank variable is recomputed when the Range variable changes, so that same fraction of range is maintained. Doubling, or halving the Range variable, doubles or halves the Blanking variable, respectively.</p> |
| Temp      | The Temp variable displays the sensor temperature in degrees Celsius. Due to the internal heating effect of the sensor, the reading may appear low when the transmitter is initially powered on. Allow at least 30 minutes for the reading to stabilize.                                                                                                                                                                                                                                                                                                 |

**Sensor Cal History (Link)**

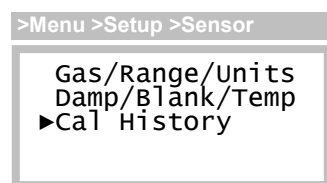

*Figure 29. Sensor Cal History*


**Table 12. Sensor Cal History**

| Variables   | Description                                                                              |
|-------------|------------------------------------------------------------------------------------------|
| Cal_History | Cal_History is a link to the Calibration History page (see Sensor Calibration Records ). |

<sup>3</sup> T90 is the time required for the transmitter to reach 90% of its final value, after a step change in gas concentration.


## Bump-Testing

“Bump-testing” refers to a test whereby the sensor is briefly exposed to gas in order to verify the reading moves upscale from zero. It is recommended that it be performed at least once a month, using a small amount of bottled span gas.

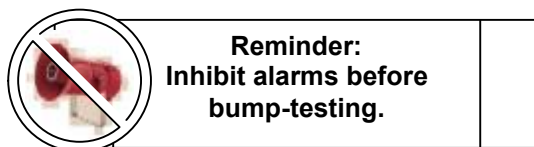

Exposing the sensor to any reactive gas could cause false alarms, and can be avoided by temporarily inhibiting them. The most convenient method for doing so is from the Main Display, using the Esc key. This also allows you to view the transmitter reading to verify the sensor’s response.

### *To quickly inhibit alarms...*

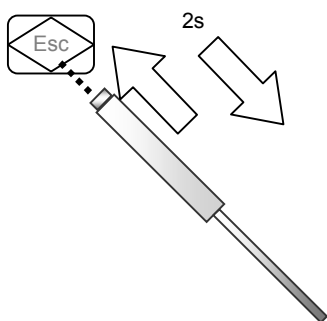

Hold the magnet over the ESC key for 2 seconds, and remove it. This will toggle the alarm inhibit mode on for 15 minutes (default value), hold the current loop at 4mA, and cause the “I” and “L” status indicators to appear. Repeat the procedure when finished with the bump-test, and verify the flags disappear. See “Inhibiting Alarms” for more details.

## **Calibration**

### **Calibration Frequency**

While the EXP-SNR transmitter requires no periodic calibration, it is recommended that the IR sensors be zero and span calibrated every 3-6 months. The frequency of calibration may depend on environment factors. Sensors frequently exposed to dirt, oil mist, vapors, or very dry air, may require more frequent calibration.

### **Calibration Terminology**

The zero calibration is referred to as, “zero”, “zeroing”, and “zeroed”. Likewise for the span calibration, which appears as, “span”, “spanning”, and “spanned”. IR sensors have an inherently non-linear response to gas that causes zero errors to magnify span errors. Therefore, zero calibration must be performed before span. Further, an appropriate bottled zero gas source must be used to zero, if span is to be performed.

### **Zero Calibration**

As the name implies, zero calibration corrects the transmitter reading to zero in the absence of any gas that causes a response by the sensor. During zero calibration, the transmitter offset error is stored and subsequently used to normalize readings.

HC and HHC IR sensors may be zero calibrated to the atmosphere under the following conditions.

- a) the atmosphere is known to be free of hydrocarbon gases
- b) the sensor will not be subsequently span calibrated

If either of the above is not true, HC and HHC sensors must be zero calibrated with bottled zero air, or nitrogen (N<sub>2</sub>). CO<sub>2</sub> and N<sub>2</sub>O IR sensors must always be zero calibrated with bottled nitrogen.

### **Span Calibration**

The role of span calibration is to correct the transmitter reading to a known concentration of target gas. During span calibration, the transmitter stores the response of the sensor and uses it to compute subsequent readings. As mentioned above, zero calibration with a bottled zero gas source must be performed before span.

### **Calibration Kits**

Bottled calibration kits containing calibrated zero and span gases are available from . Contact , or your local representative, if you have questions about calibration gas kits or gas sources.

### **Indications During Sensor Calibration**

The “un-blanked” gas concentration value is displayed during zero and span calibration, primarily to observe any slight amount of positive or negative drift. In addition, alarms are cleared and inhibited, and the 4-20mA output of the EXP-SNR transmitter is locked at 4.0mA. The 4-20mA output will not change when gas is applied and removed, and for 15 minutes thereafter (the default value). While viewing the calibration pages, the LCD display will indicate the changing gas concentration.

### **Calibration Exceptions**

Zero and span calibration are not allowed during the following conditions:

- ❖ transmitter is in the 5-minute<sup>4</sup> warm-up period
- ❖ a transmitter fault is active

To help prevent calibration errors, zero and span are not allowed if the sensor output, or span value entered, is too high or too low.

### Series EXP-SNR Gas Transmitter with IR Sensor

#### Zero Calibration with a Zero Gas Source


In addition to the bottled zero gas source, you will need a 500 cc/min regulator, calibration adapter, and a convenient length of 1/4" tubing. Referring to Figure 30, screw the calibration adapter onto the exposed end of the sensor and connect one end of the tubing (1), connect the other end of tubing to the cylinder's regulator (2). Do not open the gas valve until instructed and skip to the Zero Sensor Page below.

#### Zeroing to the Atmosphere

This procedure is permitted only for HC and HHC IR sensors, providing that:

- the atmosphere is known to be free of hydrocarbon gasses, and,
- span calibration will not be subsequently performed

Continue with the Zero Sensor Page below.

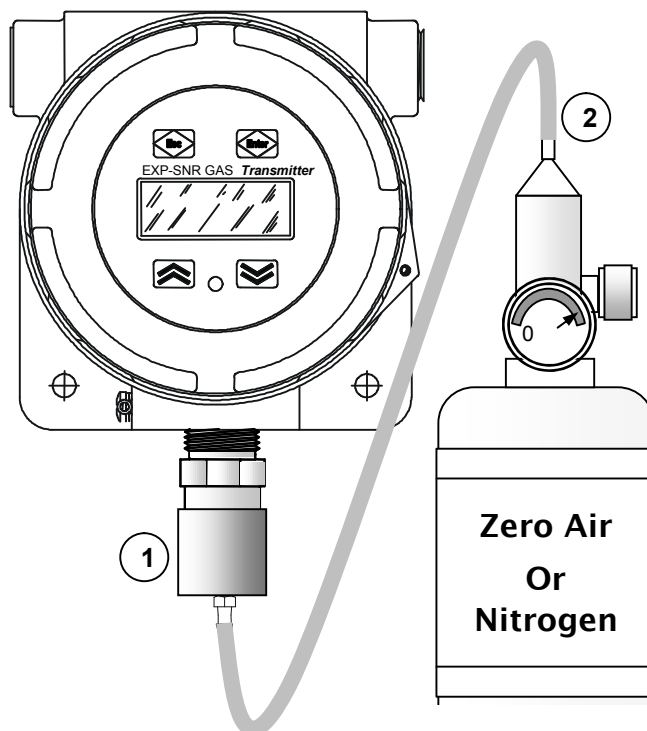


*Figure 30. Zero calibration*

#### Zero Sensor Page

From the Main Display, select Menu, then Zero\_Sensor, as shown in

Figure 31. This will clear and inhibit alarms at the transmitter, and hold the current loop output at 4mA.

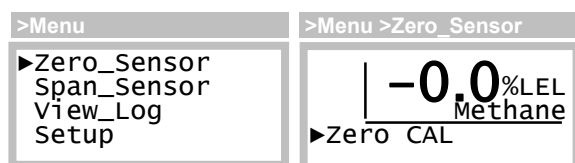

*Figure 31. Zero Sensor page*

Open the regulator to flow gas to the sensor. After approximately four minutes, select Zero. The "Cal" message will appear at the bottom of the page and remain while the transmitter adjusts its input amplifier circuitry. When finished with the adjustment, the reading will be forced to 0. Since the reading is not blanked, it may show a negative indication, like "-0", which is normal.

Touch the Escape key twice to leave the Zero\_Sensor page and return to the Main page. By default, alarms will remain inhibited, and the current loop fixed for 15 more minutes (the default value).

**Series EXP-SNR Gas Transmitter with IR Sensor**


**Span Calibration Procedure**

Span calibration\* requires a cylinder of “span” gas with a 500 cc/min regulator, calibration adapter, and a convenient length of 1/4” tubing. Referring to


Figure 32, screw the calibration adapter onto the exposed end of the sensor and connect one end of the tubing (1) to it, connect the other end of tubing to the cylinder’s regulator (2). Do not open the gas valve until instructed below.

\* Perform the Zero calibration prior to the Span calibration.

From the Main Display, select Menu, then Span\_Sensor, as shown in Figure 33. This will clear and inhibit alarms at the transmitter, and hold the current loop output at 4mA.

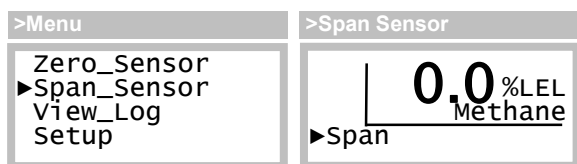


*Figure 33. Span Sensor page*

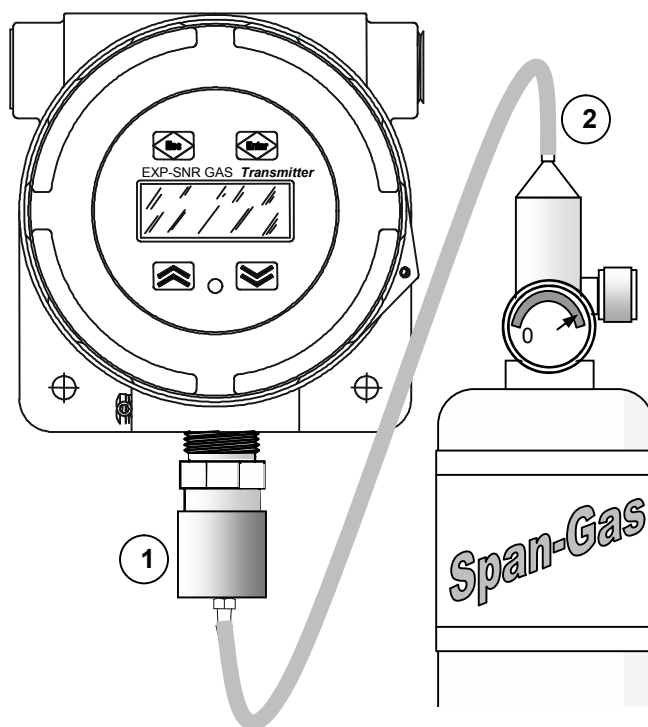

*Figure 32 Span calibration*

Open the regulator and allow span gas to flow to the sensor. Observe the displayed reading begins to increase, and at the end of four minutes, the reading should be stable.

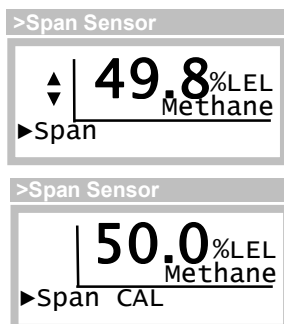

Select Span, the concentration reading will become fixed, and the blinking Up/Dn edit cursor will appear just to the left of the reading. Touch the Up or Down key to correct the reading to match the known concentration of gas, then touch Enter.

The ‘Cal’ message will appear briefly at the bottom of the page. The procedure may be cancelled by selecting Undo. The Undo function is only possible while remaining on the Span\_Sensor page. Leaving the page will disable the possibility of canceling the span calibration.

Touch the Escape key twice to leave the Span\_Sensor page and return to the Main page. Disconnect the calibration adapter from the sensor and permit the readings to return to zero. By default, alarms will remain inhibited and the current loop fixed for 15 more minutes (the default value). Once the reading is below any of the alarm set points, you may terminate the alarm inhibit (and fixed loop output) using the Esc key on the Main Display (see Esc Key Operation - Main Display in the Main Display Page section).


**Series EXP-SNR Gas Transmitter with IR Sensor**

**Spanning for Safety – HC and HHC IR Sensors**

It is usually best to avoid situations where the HC or HHC IR sensor may be exposed to more than one combustible gas at the same time, due to differences in LEL and sensitivity. In situations where it cannot be avoided, calibrate the sensor to the gas exhibiting the lowest sensitivity at its corresponding LEL. This will provide the highest margin of safety. Although a false alarm may result if a leak develops by one of the other gases, this strategy safeguards against potentially explosive conditions developing at the sensor location. Contact the factory for information about the sensitivity of IR sensors.

## **Sensor Calibration Records**

A calibration record is written into the sensor memory each time a zero or span calibration is performed. Enough memory is reserved for 63 zero calibrations and 63 span calibrations. After that, new calibration records overwrite older ones (ie, 64 replaces 1, 65 replaces 2, and so on). Zero and span calibration records are accessed from the Cal\_History page as shown below.

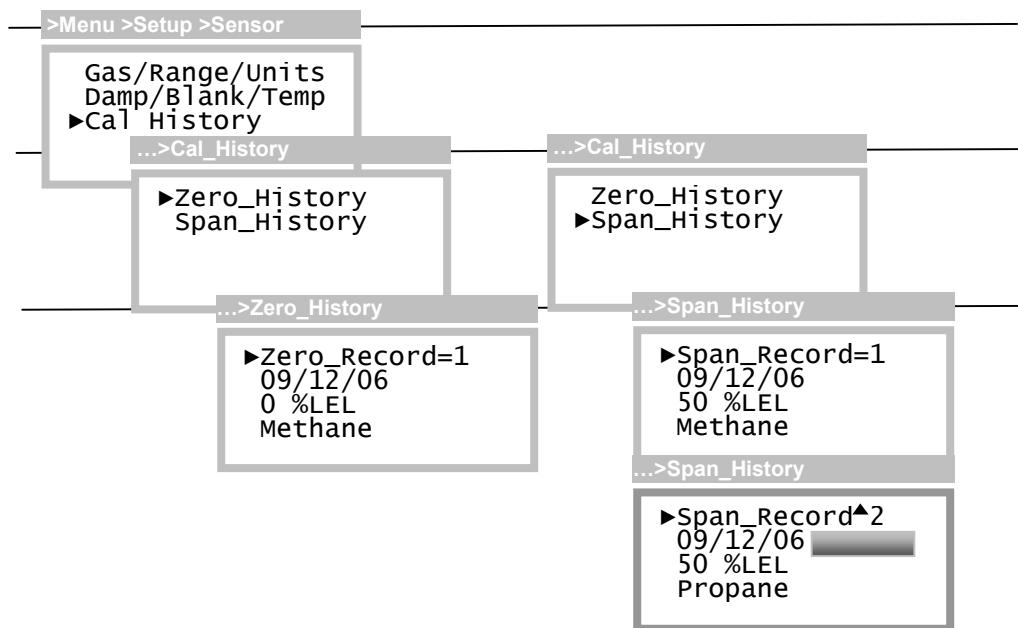

*Figure 34. Sensor calibration history pages*

Zero calibration records are accessed in the Zero\_History menu and include the index, date, and concentration reading just prior to calibration. The concentration reading is displayed in the currently programmed units, and can be thought of as the sensor “drift” from the previous zero calibration. The target gas at the time of the calibration is also displayed. Upon entry, the index number is set to the most recent calibration and may be scrolled down to view earlier calibration records.

Span calibration records are accessed in the Span\_History menu and include the index, date, and concentration of span gas used during calibration, in the currently programmed units. The target gas at the time of the calibration is also displayed. If the gas was used to calibrate a group of other gasses, the word “Group” appears as shown. Like the zero records, the index number is set to index the most recent calibration and may be scrolled down to view earlier calibration records.

## **ALARMS and RELAYS**


The standard EXP-SNR transmitter features three gas alarms, and one fault alarm. The alarm status indicators appear on the Main Display, and status is available over the optional Modbus® or HART® serial interface. Alarms may be assigned to activate one or more of the three optional relays, which are discussed below in Alarm Relays.

### **Gas Concentration Alarms**

The gas alarms are labeled, Caution, Warning, and Alarm. Although not strictly enforced, Alarm usually has the highest priority, followed by Warning and Caution. Figure 35 depicts the default relationship between the alarms.


For combustible gasses, no alarm may be set higher than 60 %LEL. The default setting for the Warning alarm is 20 %LEL, and 50%LEL for Alarm. Caution is used to alarm on negative drift of -10 %LEL or more (a fault alarm occurs if the reading drifts to -20 %LEL, or below).

*Figure 35. Default alarms for combustible gas sensors.*

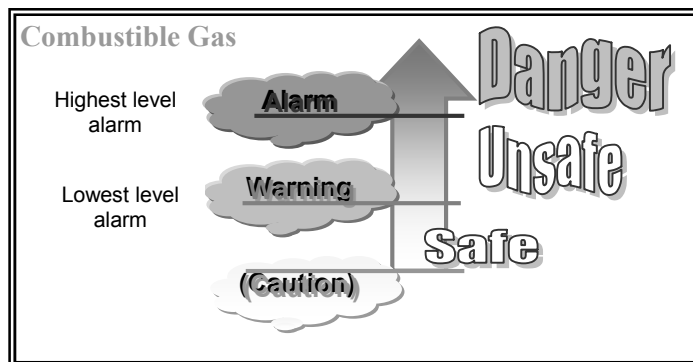

### **Manual Alarm Reset**

Alarms programmed for manual reset (see below) are held active, or latched, even after alarm conditions have subsided. On the combustible sensor version of the transmitter, Alarm is always programmed for manual reset. Latched alarms are reset from the Main Display page by selecting the respective flag (A, W, or C). The Alarm Reset page appears and displays the date and time of the alarm. If alarm conditions have subsided, you may reset just the selected alarm (Reset), or all alarms (ResetAll). A link to the Alarm Inhibit page is provided for convenience.

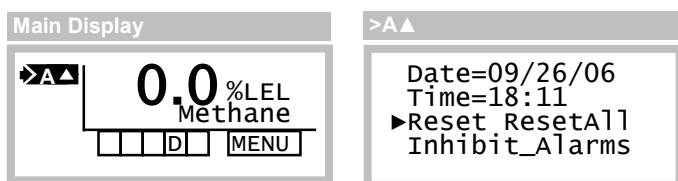

*Figure 36. Manual alarm reset*

### **Remote Reset**

Grounding the "Remote Reset" input resets all latched alarms, if the respective alarm conditions have subsided (see Figure 9. Power supply board connections.).

**Gas Alarm Setup Pages**

Variables for the gas alarms are configured on the respective setup pages, as shown in Figure 37, and described in Table 13.

|                                                                                                      |                                                              |                                                              |
|------------------------------------------------------------------------------------------------------|--------------------------------------------------------------|--------------------------------------------------------------|
| <div><div>►Alarm<br/>Warning<br/>Caution<br/>Inhibit</div><div>Relays<br/>Setup<br/>Test</div></div> |                                                              |                                                              |
| >Alarm                                                                                               | >Warning                                                     | >Caution                                                     |
| Active=ABOVE_SP<br>Set_Point= 50<br>Res_Point= 50<br>►More                                           | Active=ABOVE_SP<br>Set_Point= 20<br>Res_Point= 20<br>►More   | Active=BELOW_SP<br>Set_Point= -10<br>Res_Point= -10<br>►More |
| >Alarm >More                                                                                         | >Warning >More                                               | >Caution >More                                               |
| ►Reset=MANU<br>Fault_Goto=HOLD<br>Set_Delay=0                                                        | ►Reset=AUTO<br>Fault_Goto=HOLD<br>Set_Delay=0<br>Res_Delay=0 | ►Reset=AUTO<br>Fault_Goto=HOLD<br>Set_Delay=0<br>Res_Delay=0 |

*Figure 37. Alarm setup pages (example)*

**Table 13. Alarm variables**

| <b>Variable</b> | <b>Description</b>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                             |
|-----------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Active          | The Active variable is used to specify the concentration range where the alarm is active. When set to ABOVE_SP, the alarm becomes active at and above the set point (referred to as a rising alarm). When set to BELOW_SP, the alarm becomes active at and below the set point (referred to a falling alarm). Setting the value to DISABLED permanently deactivates the alarm. The variable setting is stored in the transmitter memory.                                                                                                                                                                                                                                                                                                                                                                       |
| Set_Point       | The Set_Point variable defines the concentration level that the alarm becomes active. The alarm becomes active immediately if the set delay variable is 0, otherwise, it becomes active at the expiration of the set delay period. When the set point is reprogrammed, the reset point value is also reprogrammed to the same value.                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |
| Res_Point       | <p>The Res_Point variable defines the concentration level that the alarm becomes inactive. Once the alarm is active, it will remain active until the concentration level reaches the reset point. The alarm then becomes inactive immediately if the set delay variable is 0, otherwise, the alarm becomes inactive at the expiration of the reset delay period (only if the reset variable is programmed as AUTO – see below). The limits for the reset point are defined below.</p> <p>Active=ABOVE_SP<br/>Upper limit = current set point value<br/>Lower limit = lowest set point value</p> <p>Active=BELOW_SP<br/>Upper limit = highest set point value<br/>Lower limit = current set point value</p> <p>When the set point is reprogrammed, the reset point value is reprogrammed to the same value.</p> |


---

|            |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                            |
|------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Reset      | <p>The Reset variable defines how the alarm is permitted to transition from active, to inactive. When the variable is set to AUTO, the alarm will transition without operator intervention, as soon as conditions permit (concentration reaches the reset point, and the reset delay period expires). When the variable is set to MANU, the reset conditions must prevail, and an operator must acknowledge the alarm manually, through the operator interface, the serial interface, or through the remote reset (see Electrical Connections, page 16). On the combustible sensor version of the transmitter, Alarm is restricted to MANU only.</p> <p>Note: Res_Delay is operational for AUTO only. Setting the Reset variable to MANU suppresses display of the Res_Delay variable.</p> |
| Fault_Goto | <p>The Fault_Goto variable specifies alarm behavior during transmitter faults, and overrides all other alarm settings. If the fault alarm should become active, you may program the concentration alarm to behave in one of three ways:</p> <p>HOLD - the transmitter will attempt to hold the alarm in its current state. If the alarm is active, it will remain active. If the alarm is inactive, it will be inhibited from becoming active until after the fault is cleared.</p> <p>SET - activates the alarm immediately, the set delay period is ignored. This feature permits the alarm to signal both concentration and fault conditions.</p> <p>RESET – deactivates the alarm immediately, the reset delay period is ignored.</p>                                                  |
| Set_Delay  | <p>The set delay variable is used to configure the amount of time in seconds that the concentration must be in the alarm active region before becoming active. It may be used to avoid triggering alarms on relatively short gas exposures. Also, it may be used to help prevent alarm relay chattering when the concentration level is varying between the set point and reset point. The variable may be programmed between 0 (its default) and 10 seconds.</p>                                                                                                                                                                                                                                                                                                                          |
| Res_Delay  | <p>The reset delay variable is only displayed when the Reset variable is set to AUTO. It is used to configure the amount of time in seconds that the concentration must be in the alarm inactive region before becoming inactive. Like the set delay variable, it may be used to help prevent alarm relay chattering and is preferred over using set delay. The variable may be programmed between 0 (its default) and two hours (7200 seconds).</p>                                                                                                                                                                                                                                                                                                                                       |

---


**Alarm Variable Functions**

Figure 38 depicts relationships between variables associated with a rising gas alarm, and how they function in the presence of a gas leak, and recovery.

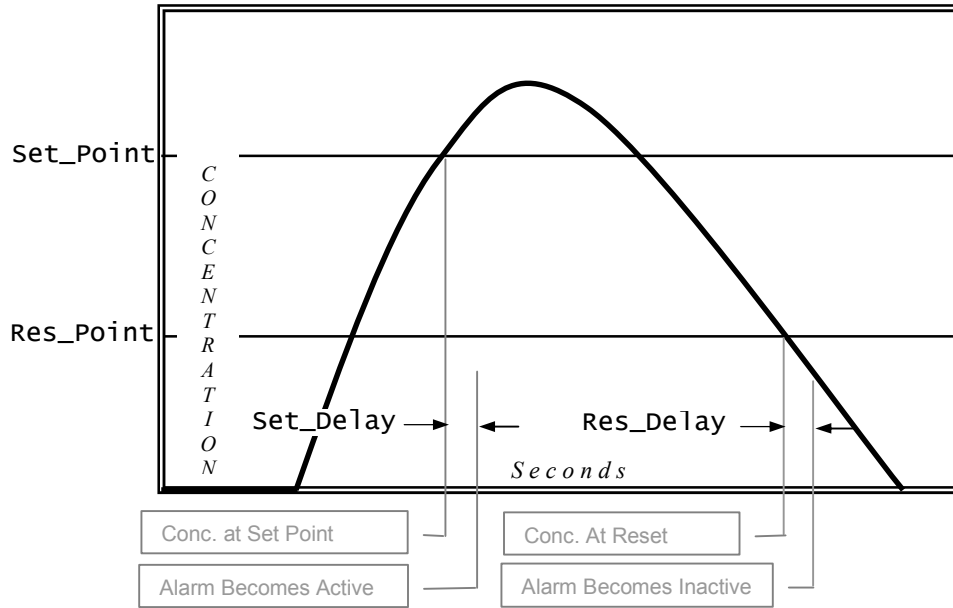

*Figure 38. Rising alarm (Active=ABOVE SP, Reset=AUTO)*


Figure 39 depicts relationships between variables associated with a falling gas alarm (such as for Oxygen deficiency), and how they function in the presence of a gas displacement, and recovery.

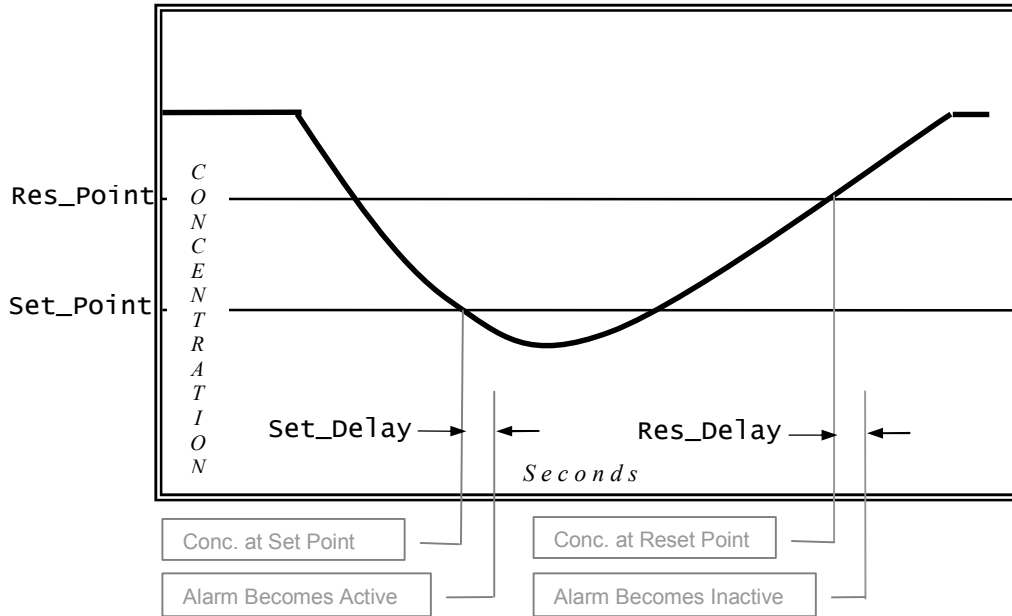

*Figure 39. Falling alarm (Active=BELOW SP, Reset=AUTO)*


## **Fault Alarms**

When a fault alarm occurs, the Main Display appears as shown below. By default, new alarms are inhibited, and active alarms are held so that relays controlling lights, sirens, and fans may continue to operate (this behavior may be modified on the Alarms Setup pages). Faults are permitted to clear automatically, without operator intervention, if they do not persist.

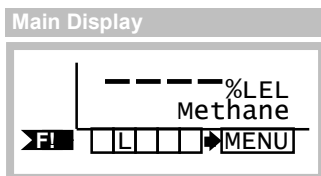

*Figure 40. Fault alarm (Main Display)*

Selecting the fault alarm flag causes the transmitter to display the fault code on line 1, and a description of the problem(s) on line 2. Selecting the Next function causes line 2 to display the next fault, if any.

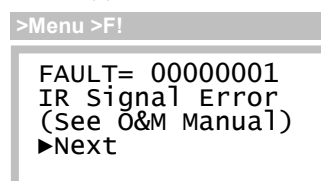

*Figure 41. Fault page*

## **Corrective Actions**

Improper wiring, ground loops, power supply sizing, current loop receivers, and other external factors may cause transmitter faults.

1. At power on, transmitters can demand 2 or 3 times the normal amount of supply current. If the supply is not sized properly, transmitters may not power on, or may produce a fault in the external power supply. If this is suspected, try starting transmitters one at a time using switch SW5 on the CPU Board.
2. Check that each transmitter has the proper supply voltage at TB1 on its Power Supply Board. The EXP-SNR Combustible Gas Transmitter requires at least 10v in all wiring modes.
3. When troubleshooting, it is permissible to temporarily swap sensors, generators, and board stacks with other transmitters. When finished, you MUST RE-VERIFY all transmitter settings, especially sensor, alarm, and 4-20mA settings. Also note that swapping components may result in losing data log records, since the log is dependent on sensor part numbers, and the full-scale range.

**Series EXP-SNR Gas Transmitter with IR Sensor**

Table 14 lists transmitter faults and corrective actions that should be attempted in the order shown. Remember to maintain safety when attempting to diagnose or perform corrective actions.



**Never enter an area, and never open a transmitter, without first making sure it is safe to do so.**

**Table 14. Fault descriptions**

| Bit No. | Fault            | Description                                                                                                                                                                                    | Corrective Action(s)                                                                                                                                                                                                           |
|---------|------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 0       | IR Signal Error  | One or both of the IR sensor signal inputs have failed, or are out of limits. This may indicate a wiring or environmental problem, or an actual failure of the sensor or transmitter hardware. | <ol style="list-style-type: none"><li>1. Cycle power</li><li>2. Re-zero the sensor</li><li>3. If remote, check sensor wiring</li><li>4. Replace upper stack</li><li>5. Replace sensor</li><li>6. Replace lower stack</li></ol> |
| 1       | LCD Busy Error   | The LCD driver chip cannot recover from an internal error.                                                                                                                                     | <ol style="list-style-type: none"><li>1. Cycle power</li><li>2. Replace upper stack</li><li>3. Replace lower stack</li></ol>                                                                                                   |
| 2       | SPI Bus Error    | Serial peripheral interface bus has faulted.                                                                                                                                                   | <ol style="list-style-type: none"><li>1. Cycle power</li><li>2. Replace upper stack</li><li>3. Replace lower stack</li></ol>                                                                                                   |
| 3       | ADC1 Read Error  | The sensor's temperature signal is out of limits, or the analog-to-digital converter channel assigned to it has failed.                                                                        | <ol style="list-style-type: none"><li>1. Cycle power</li><li>2. Replace upper stack</li><li>3. Replace sensor</li><li>4. Replace lower stack</li></ol>                                                                         |
| 4       | Sensor (-)Range  | The sensor has drifted -20% range (below zero).                                                                                                                                                | <ol style="list-style-type: none"><li>1. Zero sensor</li><li>2. Replace sensor</li><li>3. Replace upper stack</li><li>4. Replace lower stack</li></ol>                                                                         |
| 5       | Sensor Removed   | The sensor cannot be detected. This appears when the transmitter cannot detect the sensor's temperature input signal.                                                                          | <ol style="list-style-type: none"><li>1. Cycle power</li><li>2. Reconnect sensor</li><li>3. Replace sensor</li><li>4. Replace upper stack</li><li>5. Replace lower stack</li></ol>                                             |
| 6       | Sensor Mem Error | One or more configuration variables in the sensor memory failed checksum.                                                                                                                      | <ol style="list-style-type: none"><li>1. Cycle power</li><li>2. If remote, check sensor wiring</li><li>3. Replace sensor</li><li>4. Replace upper stack</li></ol>                                                              |

**Series EXP-SNR Gas Transmitter with IR Sensor**

---


|    |                  |                                                                                                                                                                   |                                                                    |
|----|------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------------------------------------------------------------------|
| 7  | Sensor Cfg Error | One or more sensor configuration variables are outside of expected range.                                                                                         | 1. Cycle power<br>2. Replace sensor<br>3. Replace upper stack      |
| 8  | Gas Gen Removed  | Not applicable to IR sensors.                                                                                                                                     |                                                                    |
| 9  | Gen Incompatible | Not applicable to IR sensors                                                                                                                                      |                                                                    |
| 10 | System Mem Error | A checksum error has been detected in the system (hardware) setup memory.                                                                                         | 1. Cycle power<br>2. Replace upper stack<br>3. Replace lower stack |
| 11 | Alarm Mem Error  | A checksum error has been detected in the alarm setup memory.                                                                                                     | 1. Cycle power<br>2. Replace upper stack<br>3. Replace lower stack |
| 12 | Operator Mem Err | A checksum error has been detected in the operator setup memory.                                                                                                  | 1. Cycle power<br>2. Replace upper stack<br>3. Replace lower stack |
| 13 | HART Mem Error   | A checksum error has been detected in the HART setup memory.                                                                                                      | 1. Cycle power<br>2. Replace upper stack<br>3. Replace lower stack |
| 14 | Autotest Failed  | Not applicable to IR sensors.                                                                                                                                     |                                                                    |
| 15 | Use 3-Wire Power | Not applicable to IR sensors (always powered in 3- or 4-wire mode)                                                                                                |                                                                    |
| 16 | UNCALIBRATED     | This appears on the Main Display, in place of the gas name, when the transmitter has not been factory calibrated, or the calibration memory has become corrupted. | 1. Cycle power<br>2. Replace upper stack<br>3. Replace lower stack |
| 17 | Stack Overflow   | An internal error occurred in the CPU program or data stack.                                                                                                      | 1. Cycle power<br>2. Replace upper stack                           |
| 18 | Fault Alarm Test | Fault alarm is being tested locally, or remotely (not a fault).                                                                                                   | No action required.                                                |
| 19 | Not Used         |                                                                                                                                                                   |                                                                    |
| 20 | Factory Cal Err  | An error has been detected in the factory calibration memory.                                                                                                     | 1. Cycle power<br>2. Replace upper stack                           |

---

**Alarm Relays**

The EXP-SNR transmitter provides three optional SPDT mechanical relays rated for 5 amps, non-inductive loads at 250VAC. These relays are suitable for switching small loads, such as horns and warning lights, but should not be used to switch motors or other high current, inductive loads.

Each relay is assigned to one of the four alarms, and may be programmed as normally energized (failsafe), or normally de-energized. A normally energized relay will have electrical continuity between its C and NO contacts (while the transmitter is powered on), and will be open between its C and NC contacts. Conversely, a normally de-energized relay will have continuity between its C and NC contacts, and will be open between its C and NO contacts. Figure 42 illustrates the function of alarm and relay variables on the operation of the relays.

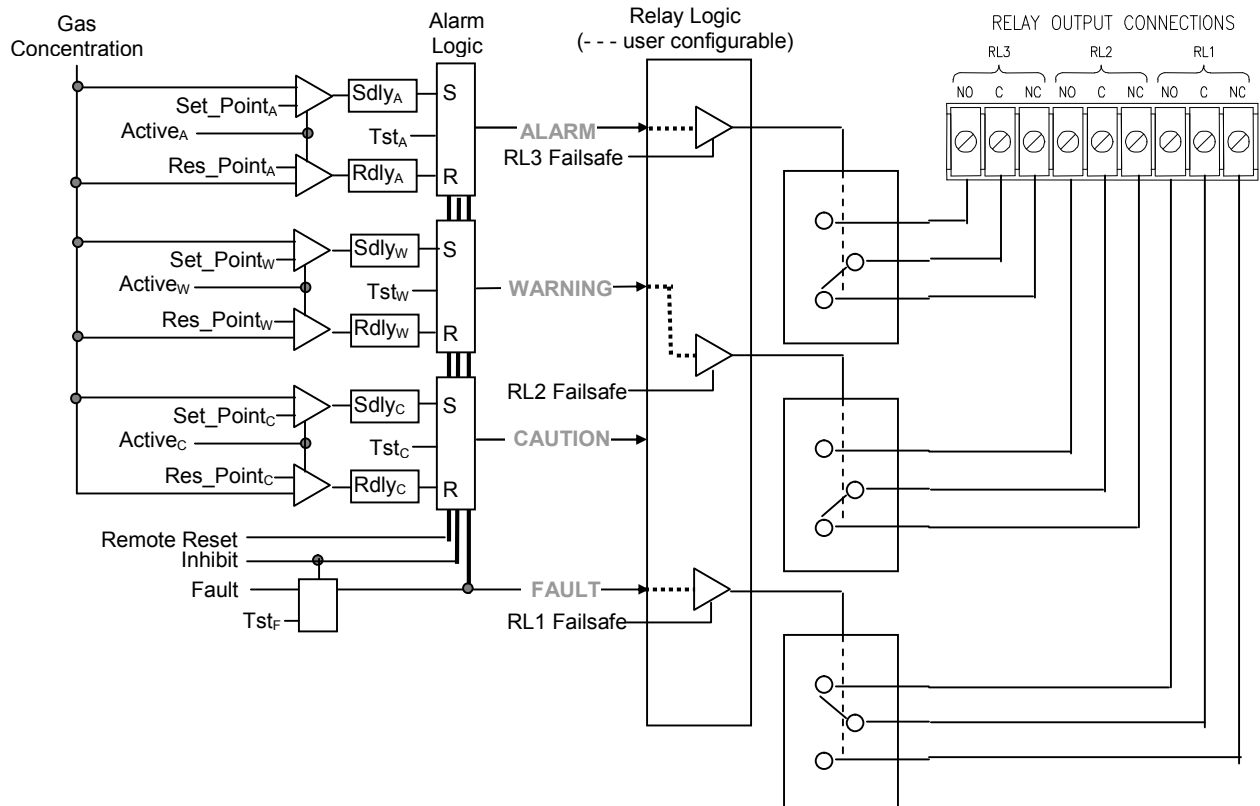

*Figure 42 Alarm relay schematic  
(default configuration – no alarms active)*

Relay Setup Page

Relays are configured in the Relays Setup page, which is accessed by selecting Menu, Setup, Alarms, and (Relays) Setup. Select the alarm trigger source (Alarm, Warning, Caution, Fault), and failsafe property (Normal-On or Normal-Off).

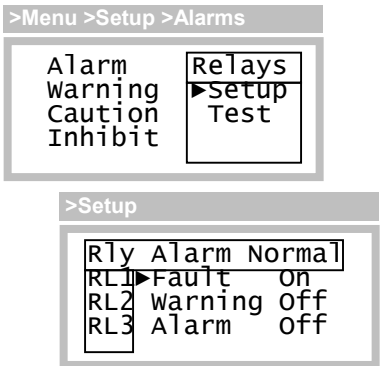


Figure 43. Relay setup page (example)

Testing Alarm Relays

Relays are tested by triggering (simulating) their assigned alarms on the Relay Test page. To trigger an alarm, scroll the “Select” variable up and down until an X appears below the letter representing the alarm. Save the selection by touching the Enter key, and move the cursor to the function labeled “Start”.

**Caution: devices wired to the relays may activate when “Start” is selected. Be sure to inform proper personnel before performing the test.**

When ready, select “Start” to begin the test. “Start” will be replaced by, “Any key to Stop”, and touching any key will end the test.

Relay Test Page

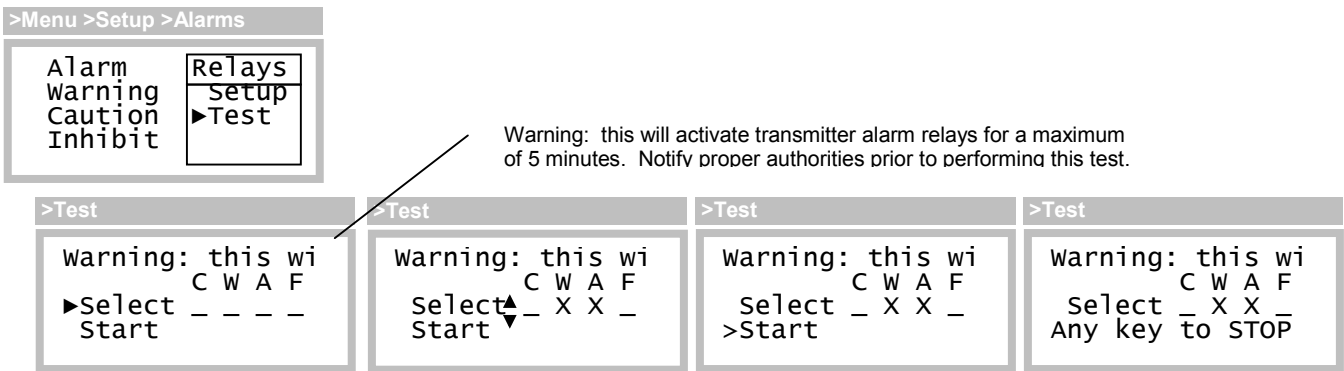


Figure 44. Relay test page example

## Inhibiting Alarms

Alarms should be inhibited to prevent false activation, such as done just prior to “bump-testing” the sensor.

The most convenient method for temporarily inhibiting alarms is from the Main Display. Hold the magnet over the ESC key for 2 seconds, and remove it. This will toggle the alarm inhibit mode on for 15 minutes, which will clear and inhibit alarms, hold the current loop at 4mA, and cause the “I” and “L” status indicators to appear. Repeating the procedure toggles alarm inhibit mode off immediately, restores the current loop to normal operation, and clears the “I” and “L” status indicators. Both the inhibit duration, and loop output, are programmable and may be accessed on the Alarm Inhibit setup page (see below).

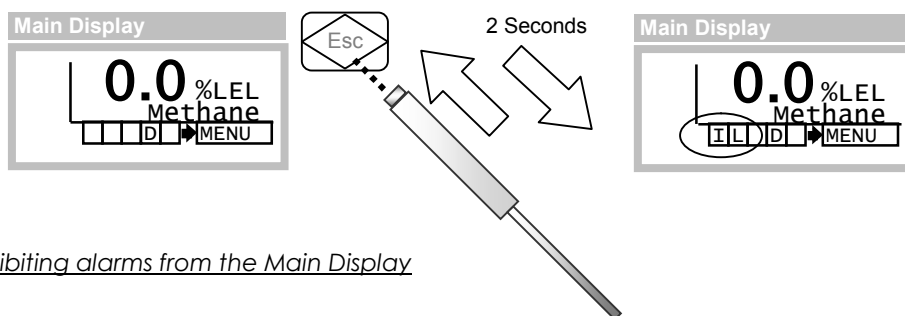


Figure 45. Inhibiting alarms from the Main Display

### Alarm Inhibit Setup page

Variables and controls associated with the alarm inhibit mode are accessible on the Alarm Inhibit setup page (below), and are detailed in Table 15.

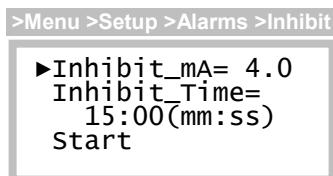


Figure 46. Alarm inhibit setup page


**Table 15. Alarm inhibit variables and controls**

| Variables    | Description                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     |
|--------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Inhibit_mA   | The Inhibit_mA variable is output on the current loop during alarm inhibit. It ranges from 3.5 to 22.0 mA (this is the same value that appears on the 4-20mA Setup page).                                                                                                                                                                                                                                                                                                                                                       |
| Inhibit_Time | <p>Alarm Inhibit Off</p> <p>The Inhibit_Time variable is the duration of the alarm inhibit mode, and is programmable from 00:00 to 99:59 (mm:ss).</p> <p>Alarm Inhibit On:</p> <p>The variable counts down from its programmed duration. Selecting it temporarily freezes the count and permits it to be scrolled up and down. If Enter is touched, counting resumes from the new value. If Esc is touched, counting resumes at the previous value. These changes are temporary, and are not saved as the programmed value.</p> |
| Start (Stop) | The Start function turns on alarm inhibit, which clears and inhibits alarms, holds the current loop at 4mA, causes the “I” and “L” status indicators to appear, and starts the Inhibit_Time variable to begin ticking down. The label then changes to “Stop”, and selecting it again turns off alarm inhibit, restore the current loop to normal operation, clears the “I” and “L” status indicators, and restores the Inhibit_Time variable to its programmed value.                                                           |

## 4-20mA Analog Output

The 4-20mA output normally sources positive current to a receiver, proportional to the main reading. The output is 4 mA at zero, and rises 20mA at the full-scale range (see “Range” variable in Sensor Target Gas, Range, Units, LEL Variables), and may go as high as 24mA (125%LEL) in case of gas flooding. Since reading is blanked below zero, the output never go below 4mA in the course of normal operation.

*Figure 47. Current loop output plot*

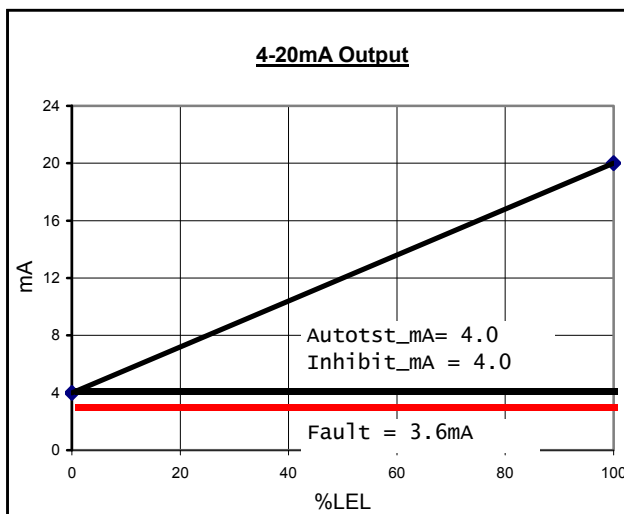


to  
and  
the  
should

### Output Overrides

By default, the output is forced to 3.6mA to signal fault alarms to the receiver. During alarm inhibit and auto-test modes, the loop is fixed at 4.0mA to prevent false alarms at the receiver. These are the default values, which may be changed on the 4-20mA Setup page.

### 4-20mA Setup Page

Variables listed on this page are described below.

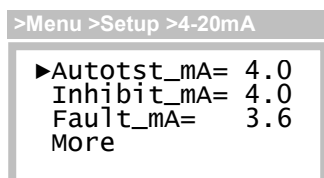

*Figure 48. 4-20mA setup page*


**Table 16. 4-20mA variables**

| Variables  | Description                                                                                                                                                                                                   |
|------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Autotst_mA | The Autotst_mA variable is the mA value output during Auto-test mode – to prevent false alarms at the receiver. The default is 4.0mA, and is limited between 3.5 <sup>5</sup> and 22.0 mA.                    |
| Inhibit_mA | The Inhibit_mA variable is the mA value output during the Alarm Inhibit mode – to prevent false alarms at the receiver. The default is 4.0, and is limited between 3.5 <sup>2</sup> and 22.0 mA.              |
| Fault_mA   | The Fault_mA variable is the mA value output during Fault alarms. The default is 3.6mA, and is limited between 3.5mA <sup>2</sup> and 22.0mA. The value should be recognized as a fault by the loop receiver. |
| More       | More is a link to the 4-20mA control page.                                                                                                                                                                    |

<sup>5</sup> Since the transmitter may be powered from the current loop, 3.5mA is the lower limit for all settings.

#### **4-20mA Control Page**

The 4-20mA Control page permits adjustment of the analog output, and provides a method for manually forcing it to a fixed value to overcome leakages, verify linearity, or test receiver alarms.

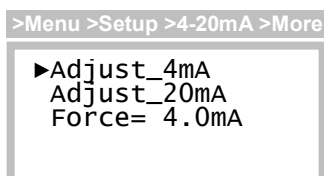

*Figure 49. 4-20mA control page*

**Table 17. 4-20mA control variables**


| Variables   | Description                                                                                                                                                                                                                                                                                                              |
|-------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Adjust_4mA  | The Adjust_4mA variable is used to adjust the 4mA level on the 4-20mA output.                                                                                                                                                                                                                                            |
| Adjust_20mA | The Adjust_20mA variable is used to adjust the 20mA level on the 4-20mA output.                                                                                                                                                                                                                                          |
| Force       | The Force variable is used to force the 4-20mA output to a fixed value. While the variable is not selected, the displayed value is updated to show the real-time output level. The loop is fixed at the instant the variable is selected, and the value may be scrolled up and down as desired, between 3.5 and 22.0 mA. |

#### **Loop Adjustment**

Loop adjustment consists of adjusting the 4 and 20 mA levels (order does not matter) by scrolling the corresponding DAC<sup>6</sup> value. This may be accomplished by reading a current meter connected across the mA(+) and mA(-) terminals of TB1 on the transmitter's Power Supply Board, or reading the display of a calibrated, current loop receiver.

|  |                                                                                   |  |
|--|-----------------------------------------------------------------------------------|--|
|  | <b>Warning:</b><br><b>Disable current loop receiver alarms before proceeding.</b> |  |
|--|-----------------------------------------------------------------------------------|--|

Select Adjust\_4mA or Adjust\_20mA and observe the following displays. Select DAC\_Value and scroll the displayed value up and down to achieve the desired output level, and touch Enter to save, or Esc to exit without saving.

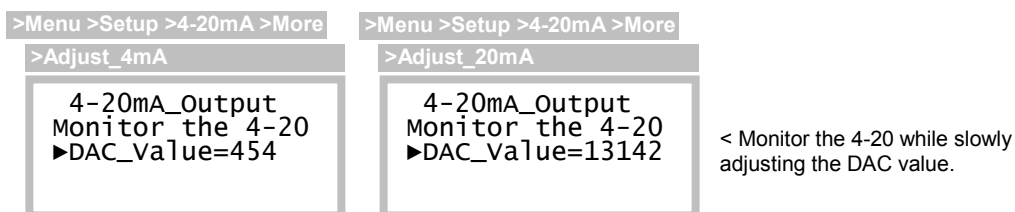

*Figure 50. Loop adjustment pages*

*(DAC values shown may not match)*

<sup>6</sup> Digital-to-Analog-Converter value ranging 0 to 16383 (14-bits). Adjustment is performed at factory, values will vary from transmitter to transmitter. This range may increase on future versions.

## **Data Logger**

The EXP-SNR transmitter data logger records gas concentration in one of 12 discrete intervals ranging from 1 to 60 minutes, providing data from 11 to 474 days. Table 18 details sampling intervals and the associated metrics.

**Table 18. Data-log sampling metrics**

| <b>Sampling<br/>(Minutes)</b> | <b>Samples/Day</b> | <b>Days</b> |
|-------------------------------|--------------------|-------------|
| 1                             | 1440               | 11          |
| 2                             | 720                | 22          |
| 3                             | 480                | 32          |
| 4                             | 360                | 43          |
| 5                             | 288                | 54          |
| 6                             | 240                | 64          |
| 10                            | 144                | 104         |
| 12                            | 120                | 124         |
| 15                            | 96                 | 152         |
| 20                            | 72                 | 196         |
| 30                            | 48                 | 278         |
| 60                            | 24                 | 474         |

Gas concentration (see

### Series EXP-SNR Gas Transmitter with IR Sensor

Main Reading) is recorded as an instantaneous value, and is not averaged or filtered in any way. When the data log memory is filled, new records will overwrite older ones.

#### Data-log Access Page

>Menu >Setup >DataLog

►Setup  
Review\_Tabular  
Review\_Graphic  
Print

The Data Log Access page provides links to pages described below.

*Figure 51. Data log access page*

#### Data-log Setup Page

>Menu>Setup>DataLog>Setup

►Sample= 1 mins  
Sample/Day=1440  
Max\_Days= 11  
Sampling=ON

The Data Log Setup page provides variables used to select one of the 12 discrete sampling intervals listed in Table 18, and a control for starting and stopping data-logging, and clearing the data log.

*Figure 52. Data log setup page*

**Table 19. Data-log setup variables**

| Variables                          | Description                                                                                                                                                                                                                                             |
|------------------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Sample,<br>Sample/Day,<br>Max_Days | These variables are used to select one of the 12 sampling intervals listed in Table 18. Each variable functions identically. Scrolling any one of the variables updates the other two. Warning: changing the sampling interval will clear the data-log. |
| Sampling                           | The Sampling variable is used to control data recording, which starts when set to ON, and stops when set to OFF. The data-log is cleared when set to CLR, after which the control is returned to its previous value (ON or OFF).                        |


Data may be displayed on the LCD graphically, or in a tabular report format. Data may also be output to a terminal, terminal program, or serial printer. Dates formats are configurable as MM/DD or DDMMM (see System Clock), and samples are displayed in the concentration units shown on the Main Display Page.

In place of numeric data samples, a report may display special text to indicate samples were unavailable, not yet sampled, or some condition prevented sampling.

**Table 20. Data log special text**

| Special Text | Description                                                                    |
|--------------|--------------------------------------------------------------------------------|
| ----         | Sample unavailable (transmitter powered off, or sample not yet recorded)       |
| FFFF         | Fault alarm active at time of sample                                           |
| TEST         | Auto-test active at time of sample (not applicable on IR sensor versions)      |
| CLNR         | Auto-clean option active at time of sample (Wet-H <sub>2</sub> S sensor, only) |
| ****         | Data is corrupted, or unreliable                                               |

**Data-log Graphic Report Page**

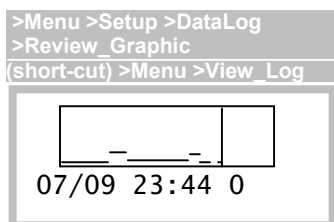


The Graphic Report page plots samples on the LCD from left to right, where older samples are on the left, and newer samples are to the right. Touching the Up and Down keys moves the vertical cursor line right and left, respectively, while updating the date, time, and sample data text on the bottom line.

*Figure 53. Data log graphic report page*

Upon entry, the cursor is parked at the most recent sample. Moving the cursor left displays the date, time, and values of earlier samples (moving it right will show “- - -”, not sampled yet). Touching the Enter key switches to the Tabular Report page, shown in Figure 54, and touching the Esc key returns to the Menu page. Data is not plotted while viewing the page.

**Data-log Tabular Report Page**

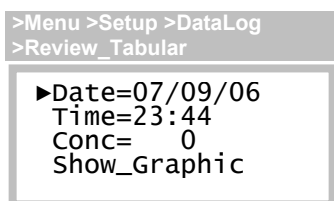

The Tabular Report page displays samples in the text field labeled “Conc”(gas concentration) and provides direct access to data by scrolling to an exact date and time.

*Figure 54. Data log tabular report page*

**Series EXP-SNR Gas Transmitter with IR Sensor**

Upon entry, the Date, Time, and Conc variables are set to the most recent sample. Scrolling the Time variable up increments it by the sampling interval, and causes the next, successive sample to be displayed at Conc. Scrolling Time down displays the previous sample time, and value. Scrolling Time up and down will cause a date rollover at midnight. Scrolling the Date variable up increments it by one day, while holding the Time variable fixed. This is an expedient method to access specific data, and is useful for examining samples recorded at the time of day.

Once the date and time are set, select the Show\_Graphic link to switch to the Graphic Report page. Data is not updated while viewing the page.

**Data-log Printout**

Data-log reports may be sent to serial printer, terminal, or terminal emulation program, such as Microsoft Hyperterminal®. See Appendix A. details on how to setup print reports.

*Figure 55. Data-log printout*

| Date     | Time  | S0   | S1   | S2   | S3   |
|----------|-------|------|------|------|------|
| 07/09/06 | 22:40 | 1    | 0    | 0    | 1    |
| 07/09/06 | 22:44 | -0   | 0    | 0    | -0   |
| 07/09/06 | 22:48 | 1    | TEST | TEST | TEST |
| 07/09/06 | 22:52 | TEST | TEST | TEST | TEST |
| 07/09/06 | 22:56 | TEST | TEST | TEST | TEST |
| 07/09/06 | 23:00 | 1    | 0    | 0    | 1    |
| 07/09/06 | 23:04 | 1    | 0    | 0    | 1    |
| 07/09/06 | 23:08 | 1    | 0    | 0    | 1    |
| 07/09/06 | 23:12 | 1    | 0    | 0    | 1    |
| 07/09/06 | 23:16 | 1    | 1    | 1    | 0    |
| 07/09/06 | 23:20 | 0    | 0    | 0    | -0   |
| 07/09/06 | 23:24 | -0   | 0    | 0    | 0    |
| 07/09/06 | 23:28 | ---- | ---- | ---- | ---- |
| 07/09/06 | 23:32 | ---- | ---- | ---- | ---- |
| 07/09/06 | 23:36 | ---- | ---- | ---- | ---- |
| 07/09/06 | 23:40 | FFFF | FFFF | 0    | 0    |

and

## Display

The EXP-SNR Transmitter features a back-lighted, 96w x 32h graphics

LCD. **Display Setup Page**

>Menu >Setup >Display

►Contrast=  
Light= MANUAL

The Display Setup page variables are used to control the display contrast, and manage the backlight.


**Table 21. Display page variables**

| Variables | Description                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                    |         |                  |        |                                                                     |      |                                                                                                              |          |                 |           |                                  |
|-----------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|---------|------------------|--------|---------------------------------------------------------------------|------|--------------------------------------------------------------------------------------------------------------|----------|-----------------|-----------|----------------------------------|
| Contrast  | The Contrast variable is used to adjust the LCD contrast. Scroll the variable up to increase contrast (darker text), or down to decrease it (lighter text). The default value is 68%, and is adjustable between 0 and 100%.                                                                                                                                                                                                                                                                                                    |         |                  |        |                                                                     |      |                                                                                                              |          |                 |           |                                  |
| Light     | The Light variable is used to control when the LCD backlighting is turned on and off. <table><tr><th>Setting</th><th>Backlight is ...</th></tr><tr><td>MANUAL</td><td>On when any key is touched<br/>Off when no key touched for 5 minutes</td></tr><tr><td>AUTO</td><td>On when any key is touched or alarm is active<br/>Off when no key touched for 5 minutes, and no alarms active</td></tr><tr><td>NEVER_ON</td><td>Off permanently</td></tr><tr><td>ALWAYS_ON</td><td>On permanently (not recommended)</td></tr></table> | Setting | Backlight is ... | MANUAL | On when any key is touched<br>Off when no key touched for 5 minutes | AUTO | On when any key is touched or alarm is active<br>Off when no key touched for 5 minutes, and no alarms active | NEVER_ON | Off permanently | ALWAYS_ON | On permanently (not recommended) |
| Setting   | Backlight is ...                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                               |         |                  |        |                                                                     |      |                                                                                                              |          |                 |           |                                  |
| MANUAL    | On when any key is touched<br>Off when no key touched for 5 minutes                                                                                                                                                                                                                                                                                                                                                                                                                                                            |         |                  |        |                                                                     |      |                                                                                                              |          |                 |           |                                  |
| AUTO      | On when any key is touched or alarm is active<br>Off when no key touched for 5 minutes, and no alarms active                                                                                                                                                                                                                                                                                                                                                                                                                   |         |                  |        |                                                                     |      |                                                                                                              |          |                 |           |                                  |
| NEVER_ON  | Off permanently                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                |         |                  |        |                                                                     |      |                                                                                                              |          |                 |           |                                  |
| ALWAYS_ON | On permanently (not recommended)                                                                                                                                                                                                                                                                                                                                                                                                                                                                                               |         |                  |        |                                                                     |      |                                                                                                              |          |                 |           |                                  |

## System

System pages provide version information and configure the internal clock, security access, communication protocols, and to reset various memory defaults.

### System Access Page

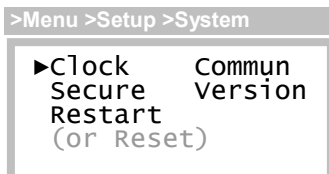


The System Access page provides links to the clock, security, communications, and version pages (the Reset link has been replaced with the Restart function on transmitters beginning with version 2.23).

*Figure 56. System access page*

## Real-time Clock

### Clock Setup Page

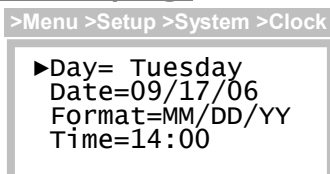


The Clock Setup page is used to set the transmitters real-time clock, which is referenced during sensor calibrations and data logging, and used to trigger Auto-test.

*Figure 57. Clock setup page*


| Variables | Description                                                                                                                          |
|-----------|--------------------------------------------------------------------------------------------------------------------------------------|
| Day       | Monday, Tuesday, Wednesday, Thursday, Friday, Saturday, and Sunday                                                                   |
| Date      | Used to configure the month, date, and year, in the format specified by the Format variable (below). Built-in support for leap year. |
| Format    | Selects the date format:<br>MM/DD/YY, example: 09/19/06<br>DDMMMYY, example: 09Sep06                                                 |
| Time      | 24-hour format, 00:00 to 23:59                                                                                                       |

Security

The transmitter protects its configuration using a 4-digit, numeric password, from 0000 to 9999. When security is active, the “S” status indicator appears on the Main Display, variables may be read, but not modified, and functions will not execute, including the sensor verification function during startup review.



Security Control Page

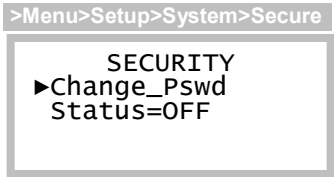

Security is off by default, and may be toggled on and off by entering the 4-digit password.

Figure 58. Security control page

Activating Security

Select the Status variable on the Security Control page, which doubles as a link to the Password Entry page. When the page appears, select Enter Pswd, scroll to the password value (0 by default), and touch Enter. If successful, “PASS” appears briefly and you are returned to the Security Control page where the Status variable is set to ON. If not successful, “FAIL” appears and Status remains OFF.

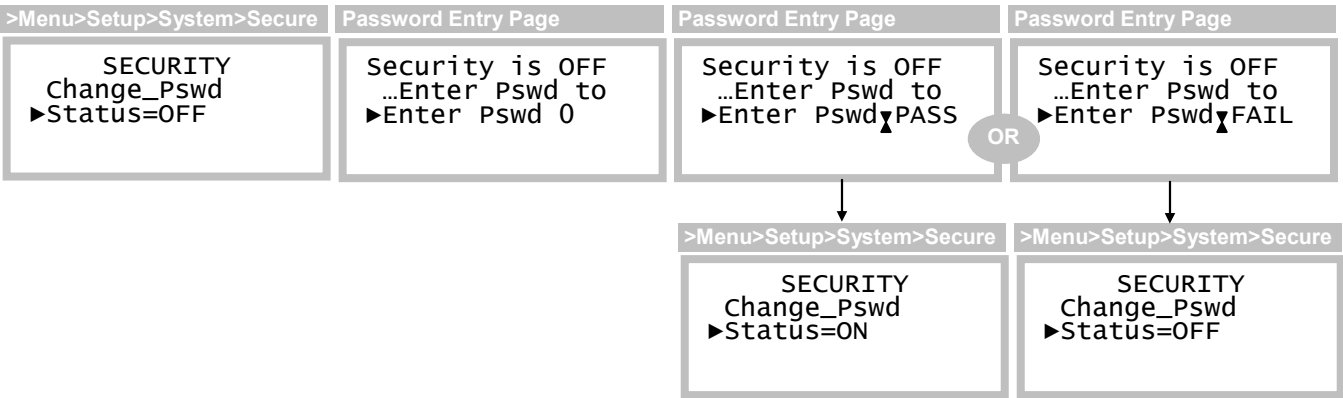


Figure 59. Activating security

### **Deactivating Security**

The procedure to deactivate security is identical to that used for activating it, and if successful, the transmitter presents an option to automatically reactivate it after a timed interval.

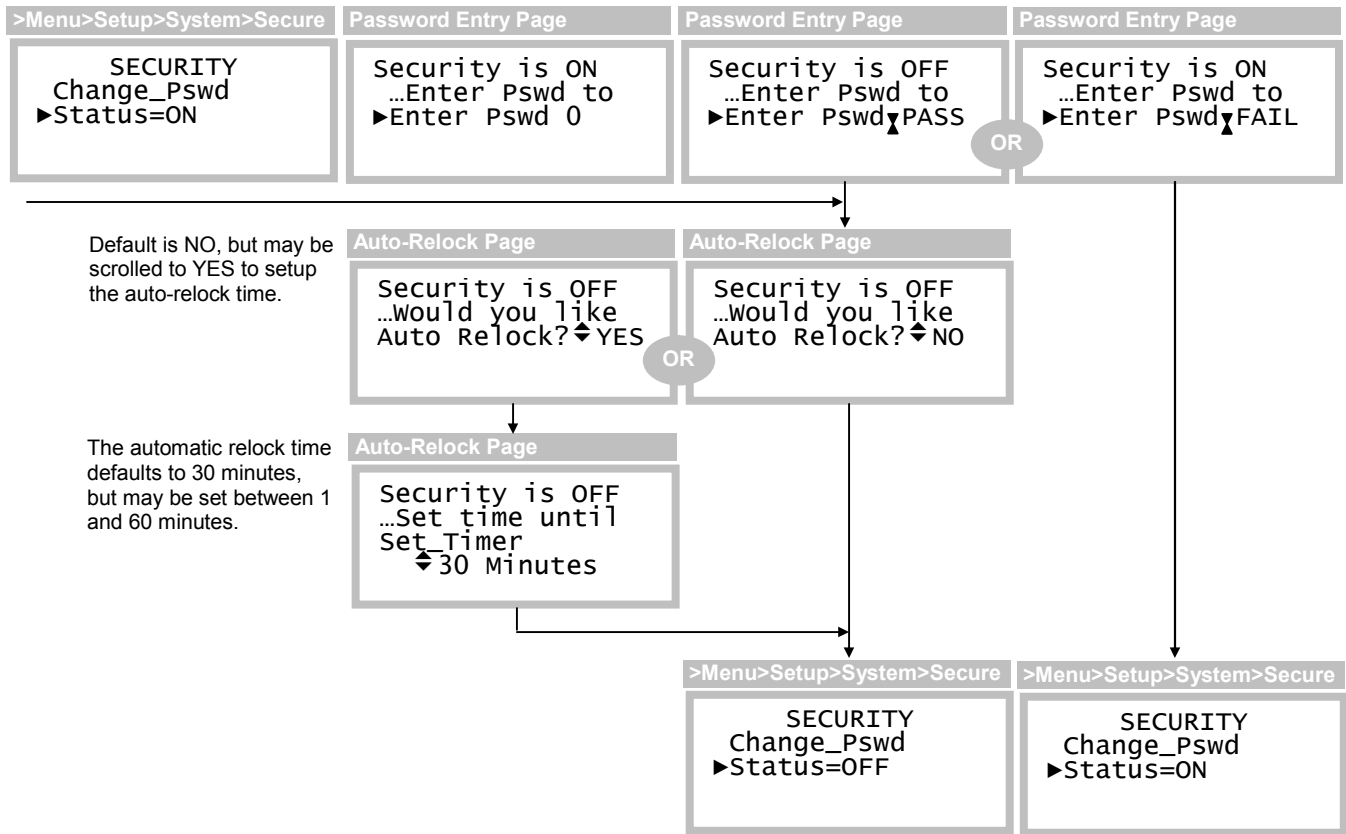


Figure 60. Deactivating security

### **Changing the Password**

The security password is changed by selecting Change\_Pswd from the Security Control page. Start by entering the old password, then enter the new one, and repeat it.


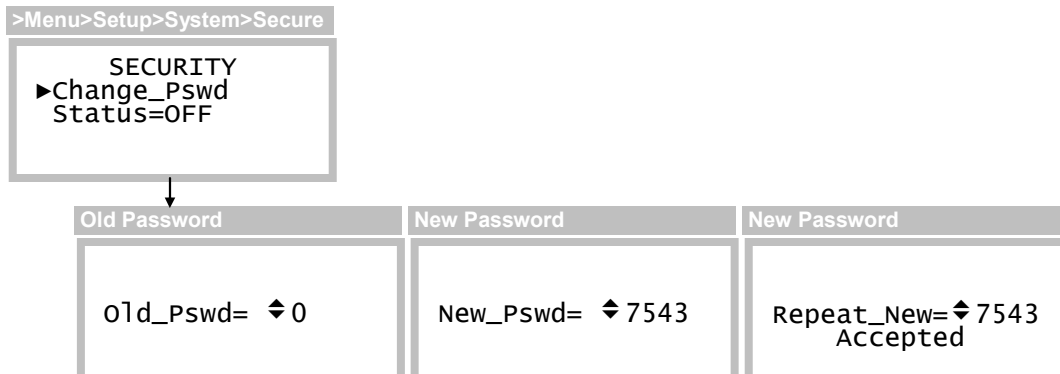


Figure 61. Changing the password

## Communications

The EXP-SNR Transmitter supports ASCII, HART 5, and Modbus communications. ASCII is the default protocol if the HART or Modbus option is not ordered.

### Communication Setup Page

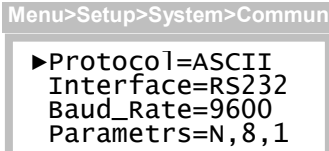

Menu>Setup>System>Commun  
►Protocol=ASCII  
Interface=RS232  
Baud\_Rate=9600  
Paramtrs=N,8,1

Communication Setup page variables are used to configure the protocol and settings of the physical communication interface. The protocol selection is performed at the factory, and may not be changed. Settings for the physical communication interface may be changed for ASCII and Modbus protocols, however, they are restricted for the HART protocol).

*Figure 62. Communication setup page*

**Table 22. Communication setup variables**

| Variables | Description                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                  |
|-----------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Protocol  | The Protocol variable identifies the installed protocol driver: <ul style="list-style-type: none"><li>• None</li><li>• ASCII (default)</li><li>• Modbus (option)</li><li>• HART (option)</li></ul>                                                                                                                                                                                                                                                                                                           |
| Interface | <p>The Interface variable selects the physical communication interface that the transmitter will control during transmit and receive functions:</p> <ul style="list-style-type: none"><li>• RS232 (available for ASCII or Modbus, not for HART)</li><li>• RS485 (available for ASCII or Modbus, not for HART)</li><li>• MODEM (available for HART only)</li></ul> <p>The transmitter must be wired in accordance with this selection (see ELECTRICAL CONNECTIONS starting on page 16).</p>                   |
| Baud_Rate | <p>The Baud_Rate variable is used to configure the baud rate of the transmitter's UART, and may be set to: 300,600,1200,2400,4800,9600,14.4k, or 28.8k</p> <p>The value is fixed at 1200 for HART protocol, and defaults to 9600 for Modbus and ASCII.</p>                                                                                                                                                                                                                                                   |
| Paramtrs  | <p>The Paramtrs variable is used to configure parity, the number of data bits, and number of stop bits of the transmitter's UART:</p> <ul style="list-style-type: none"><li>• N,8,1 ...no parity, 8 data bits, 1 stop bits</li><li>• N,8,2 ...no parity, 8 data bits, 2 stop bits</li><li>• E,8,1 ...even parity, 8 data bits, 1 stop bit</li><li>• O,8,1 ...odd parity, 8 data bits, 1 stop bit</li></ul> <p>The value is fixed at O,8,1 for HART protocol, and defaults to N,8,1 for Modbus and ASCII.</p> |

Protocol specific settings are configured on separate pages that are accessible from links on the Setup page, and are discussed below.


### **ASCII**

ASCII is used for sending the data log to a serial printer, terminal, or terminal program, using RS232 (RS485 might be used under certain conditions). Handshaking is XON/XOFF only, and the Communication Setup page may be used to configure the interface, baud rate, and communication variables. See RS232 Modbus, PC Capture, or Printer for connection details. There are no additional pages for protocol variables.

### **HART**

HART is a master/slave protocol that supports 1 or 2 masters, and up to 15 slave devices. Devices communicate digitally at an effective rate of 1200 baud by modulating the 4-20mA loop. Modulation is performed by a modem that conforms to the BELL 202 standard, which uses FSK (frequency shift keying), where 1200Hz represents a logic 1, and 2200Hz represents logic 0, and does not affect the loop's DC level. Connections are typically point-to-point, which enables bi-directional digital communication and preserves the transmitter's analog output signal. Up to 15 devices may be connected in a multi-drop configuration for digital communication, but requires each device to fix its output at 4mA. See HART Transmitter connection examples in ELECTRICAL CONNECTIONS on page 16, or consult the HART Foundation for additional details on connecting a HART transmitter.

When the HART protocol driver is installed, a link to the HART Setup page appears on the main Setup page.

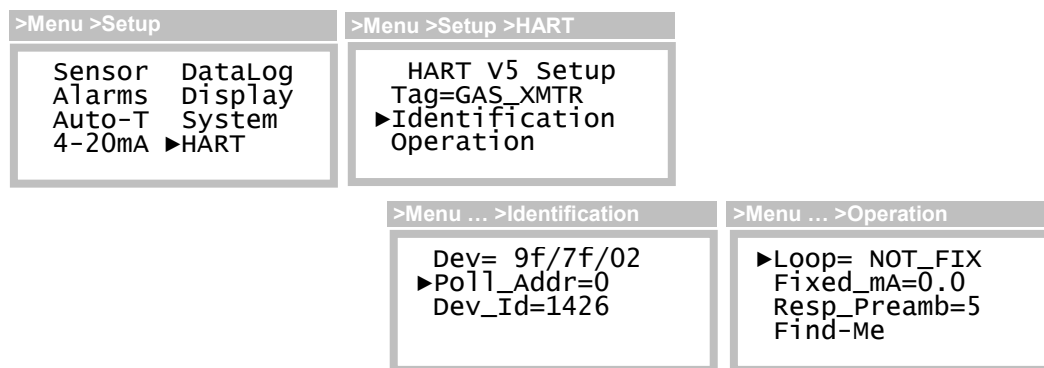

*Figure 63. Hart setup pages*

**Table 23. HART setup variables**


| Variables | Description                                                                                                                                                                                                                                                                                                                                                                                                                                                                                 |
|-----------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Tag       | The Tag variable can be used as a unique identifier for communicating to the transmitter. The variable is read only at the operator interface, but may be modified using HART network management commands.                                                                                                                                                                                                                                                                                  |
| Dev       | The Dev variable displays read-only device information used in long-frame address commands, and by devices capable of utilizing the transmitter's DDL (device description language) file. The format of the information is, MFG_ID/DEV/REV. The MFG_ID is 9f, and identifies Analytical Technology, Inc as the manufacturer. DEV is 7f, and identifies the device as a EXP-SNR transmitter. REV is the revision level of the transmitter, currently set at 2 (may increment in the future). |

---

|             |                                                                                                                                                                                                                                                                                                                                                                |
|-------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Poll_Addr   | The Poll_Addr variable sets the polling address of the transmitter. The default value is 0, which allows the transmitter to communicate digitally, while preserving the function of the 4-20mA output. The value may be set from 1 to 15, which fixes the output at 4mA, and disables analog signaling.                                                        |
| Dev_Id      | The Dev_Id variable is used to form a unique identifier in the HART long frame address. This value is set at the factory, and appears on a label attached to the transmitter. Changing this setting is not recommended.                                                                                                                                        |
| Loop        | The Loop variable specifies the operation of the 4-20mA output. When the HART polling address is 0, the value is NOT_FIX and loop functions as normal. When the address is set to 1 or higher, the value is FIXED and the output is fixed at 4mA. The ability to alter this behavior is reserved for future use, and changing this setting is not recommended. |
| Fixed_mA    | The Fixed_mA variable provides direct access the associated HART network management variable. The value is adjustable only when the Loop variable is FIXED, and may be adjusted between 3.5 and 22 mA.                                                                                                                                                         |
| Resp_Preamb | The Resp_Pream variable provides direct access to the associated HART network management variable, which determines the number of preamble characters (FF hex) transmitted at the beginning of each message. The default value is 5, and may be set from 3 to 20. Changing this setting is not recommended.                                                    |
| Find-Me     | The Find-Me function places the transmitter into the Find-Me mode, where a master device can issue a command to positively identify the physical location of the transmitter.                                                                                                                                                                                  |

---

Selecting the Find-Me function presents the special page that remains until the master device issues a “Find-Me” command to the transmitter, at which point the display changes to the “Device Found” page.

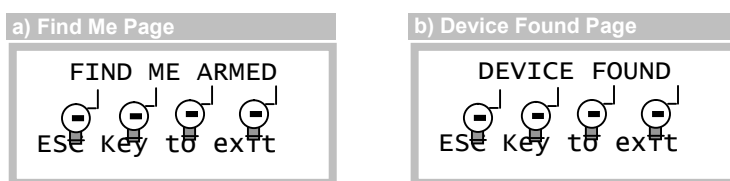


*Figure 64. Hart a) Find-me and b) Device found pages*

### **Modbus**

Modbus is a master/slave protocol that supports a single master, and up to 247 slave devices on a common bus. The RS485 interface physically limits this number to 32 (1 master, 31 slaves), and RS232 restricts communication to a master and a single slave. The Communication Setup page may be used to configure the interface, baud rate, and communication variables. See RS485 Modbus Multidrop and RS232 Modbus, PC Capture, or Printer for connection details.

When the Modbus protocol driver is installed, a link to the Modbus Setup page appears on the main Setup page.

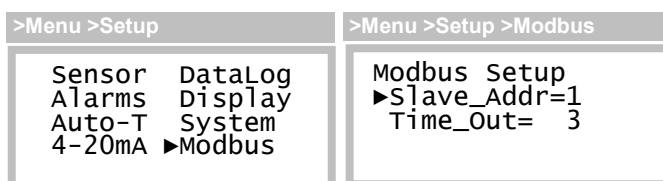


*Figure 65. Modbus setup page*

**Table 24. Modbus setup variables**

| Variables  | Description                                                                                                                                                                                                                |
|------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Slave_Addr | The Slave_Addr variable is the transmitter's slave address, which may set from 1 (default) to 247.                                                                                                                         |
| Time_Out   | The Time_Out variable belongs to the data-link layer of the protocol and defines the number of 1.5 character timeouts used to frame messages. This variable is reserved for future use and changing it is not recommended. |

### **Transmitter Version**

The Transmitter Version page displays transmitter information:

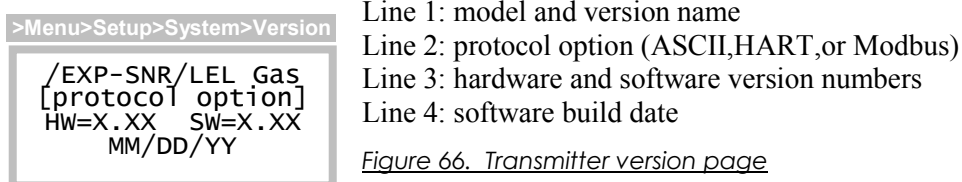

*Figure 66. Transmitter version page*


## **Restart**

The Restart function will cause the transmitter to start up, just as it does during a power-on-reset. This function replaces the Reset page beginning with version 2.23 of the EXP-SNR Combustible Gas Transmitter with Catalytic Bead sensor.

## **Resets**

Note: the Reset page has been removed on software versions 2.23, and higher.


The Reset page provides functions for resetting configuration memories, and restarting the transmitter, which may prove useful for correcting specific faults. These functions should **not be used** unless they are specified in troubleshooting procedures, or directed by authorized factory personnel.

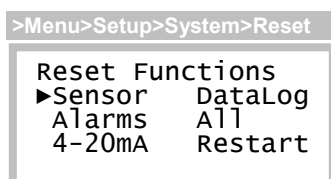

**Table 25. Reset functions (do not use except for troubleshooting).**

| <b>Function</b> | <b>Description</b>                                                                                                                                                         |
|-----------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Sensor          | Resets zero and span calibration, restarts transmitter. <u>Sensor must be completely recalibrated.</u> On LEL transmitters, calibration and Auto-test history are cleared. |
| Alarms          | Resets alarm set/reset points, options, delays, and inhibit_mA, restarts transmitter.                                                                                      |
| 4-20mA          | Resets 4-20mA calibration, loop must be recalibrated, restarts transmitter.                                                                                                |
| DataLog         | Clears the data log history, restarts transmitter.                                                                                                                         |
| All             | Resets entire transmitter to factory defaults, excluding sensor, restarts transmitter. <u>Requires full transmitter setup.</u>                                             |
| Restart         | Restarts the transmitter.                                                                                                                                                  |

## SPARE PARTS

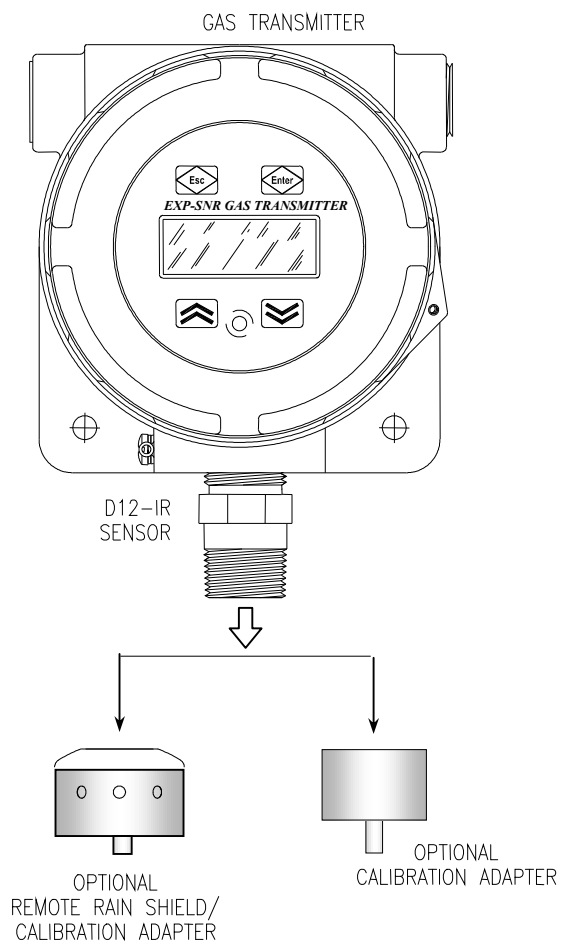

---

### Description

Standard LEL (low range) hydrocarbon sensor for Methane, Propane, Butane, Pentane, etc.

High range hydrocarbon sensor for high concentrations (normally above the UEL) of Propane, Butane, LPG.

Standard range Carbon dioxide sensor

High range Carbon dioxide sensor

Standard range Nitrous oxide sensor

EXP-SNR (3) Board Stack Assembly, Without Relays

EXP-SNR (3) Board Stack Assembly, With Relays

Remote IR Sensor Cable Assembly

Calibration adapter

Remote Calibration Adapter / Rain Shield

Battery

Magnetic Screwdriver

---

## Appendix A.


### Printing Data Log Reports

The following pages describe how to send a data-log report to a printer or computer, over a serial RS232 connection, and to import that data into Microsoft Excel for plotting.



### Serial Connection

The data log report may be sent to a printer or a computer over an RS232 connection, or in some cases, an RS485 connection.

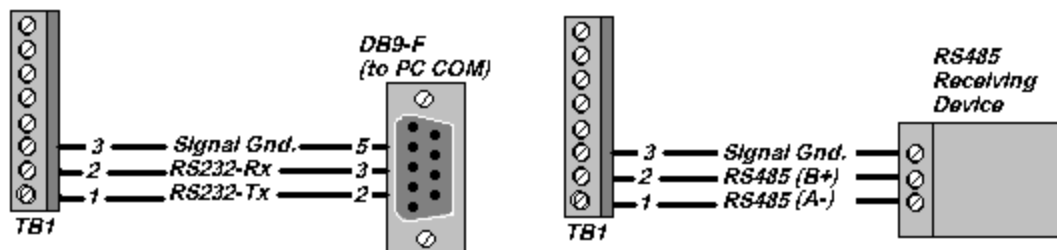

### Communication Setup Page

Menu>Setup>System>Commun

►Protocol=ASCII  
Interface=RS232  
Baud\_Rate=9600  
Parametr=N,8,1

The communication interface, baud rate, parity, number of data bits, and number of stop bits are configured on the Communication Setup page.

### Flow Control

The transmitter uses XON/XOFF flow control while sending a report. That is, once the data stream has begun, it will continue until the XOFF character (19) is received. After sitting idle, the report stream will begin again upon reception of the XON character (17).

An RS232 connection can support full duplex communication and is perfectly suited for XON/XOFF flow control. However, an RS485 connection is only half duplex. It cannot receive while it is transmitting and might miss the XOFF character, resulting in a buffer overflow at the receiving device.

A receiving device will send the XOFF character when its buffer is nearly full. Some older dot-matrix printers will send an XOFF because they have a small receive buffers and cannot process characters while the head is returning to start a new line. On the other hand, most computers have comparatively large buffers and can easily accept the report stream without sending an XOFF. Therefore, an RS485 connection may work for sending reports to a computer.

The EXP-SNR features an additional method to help avoid losing data due to buffer overflow problems on receiving devices that lack XON/XOFF capability (or have the capability but are using an RS485 connection). A programmable time delay of up to 10s may be inserted at the end of each report line. This permits the receiver time to process more characters in its buffer and avoid an overflow. However, this may be a method of trial and error until the proper delay setting is determined so that no characters are missing from the report.

## Report Format

The format of the report is suitable for import into most spreadsheet programs and consists of a date column, a time column, and 1-30 columns for sample values. Each line of the report shows the date and time of the first sample. Samples appearing in subsequent columns (left to right) were recorded at equal sampling intervals.

In the top line of the example below, the first sample (S0) occurred at 22:40. The next sample to the right (S1) occurred at 22:41, followed by the next (S2) at 22:42, and so on. This pattern is repeated throughout the report.

| Date     | Time  | S0   | S1   | S2   | S3   |
|----------|-------|------|------|------|------|
| 07/09/06 | 22:40 | 0.01 | 0.00 | 0.02 | 0.01 |
| 07/09/06 | 22:44 | -0.0 | 0.00 | 0.00 | -0.0 |
| 07/09/06 | 22:48 | 0.01 | TEST | TEST | TEST |
| 07/09/06 | 22:52 | TEST | TEST | TEST | TEST |
| 07/09/06 | 22:56 | TEST | TEST | TEST | TEST |
| 07/09/06 | 23:00 | 0.07 | 0.06 | 0.07 | 0.06 |
| 07/09/06 | 23:04 | 0.06 | 0.05 | 0.06 | 0.06 |
| 07/09/06 | 23:08 | 0.05 | 0.05 | 0.04 | 0.05 |
| 07/09/06 | 23:12 | 0.06 | 0.05 | 0.05 | 0.04 |
| 07/09/06 | 23:16 | 0.01 | 0.01 | 0.01 | 0.00 |
| 07/09/06 | 23:20 | 0.00 | 0.00 | 0.00 | -0.1 |
| 07/09/06 | 23:24 | -0.0 | 0.00 | 0.00 | 0.00 |
| 07/09/06 | 23:28 | ---- | ---- | ---- | ---- |
| 07/09/06 | 23:32 | ---- | ---- | ---- | ---- |
| 07/09/06 | 23:36 | ---- | ---- | ---- | ---- |
| 07/09/06 | 23:40 | FFFF | FFFF | 0.02 | 0.02 |

The transmitter permits selection of either a CR (carriage return) or CR/LF (carriage return/line feed) as the EOL (end-of-line) characters. If the lines of the report appear to be printing over each other, choose the CR/LF option. If the lines appear to be double spaced, choose the CR option.

The number of sample columns appearing across the page is programmable from 1 to 30. This is designed so that a report may be directed to either a small carriage printer, or to a wider format device. A wider report will take less time to print because the date and time fields will be printed less frequently.

Samples reported are assumed to be in units of PPM, PPB, %, or %LEL, as determined by the gas concentration units appearing on the main display of the transmitter. Sample values outside of printing limits are forced to the following values.

| Samples ...       | Are forced to... |
|-------------------|------------------|
| Less than -999    | -999             |
| Greater than 9999 | 9999             |

Symbols may appear in place of sample values, and are defined as follows.

| Symbol | Description                                                                                                                                               |
|--------|-----------------------------------------------------------------------------------------------------------------------------------------------------------|
| ----   | No sample recorded. The transmitter was not on to record the sample, or has not yet recorded the sample.                                                  |
| FFFF   | The transmitter was in fault during the sample.                                                                                                           |
| TEST   | The transmitter was in auto-test during the sample. This symbol appears only if the Log_Data variable in the Menu/Setup/Auto-T/Setup menu is set to "NO". |
| ****   | Data in the log is corrupted or unreliable.                                                                                                               |


## Report Control

The start date and length of the report may be controlled from the operator interface. The length of the report is limited to the number of days actually stored in the log. The report always begins at 00:00 on the start date, and continues forward for the number of days specified. If no data has yet been logged, the report will show four dashes (----) in place of samples.

## **Example: Charting a Data Log Report**

Start HyperTerminal by clicking **Start**, pointing to **Programs**, pointing to **Accessories**, pointing to **Communications**, clicking **HyperTerminal**, and then double-clicking **Hypertrm.exe**.


When the **Connection Description** dialog box appears, type in **Connect To D12**. If you wish, choose an icon by sliding the horizontal scroll bar over and clicking one of the selections. Click **OK** when ready.

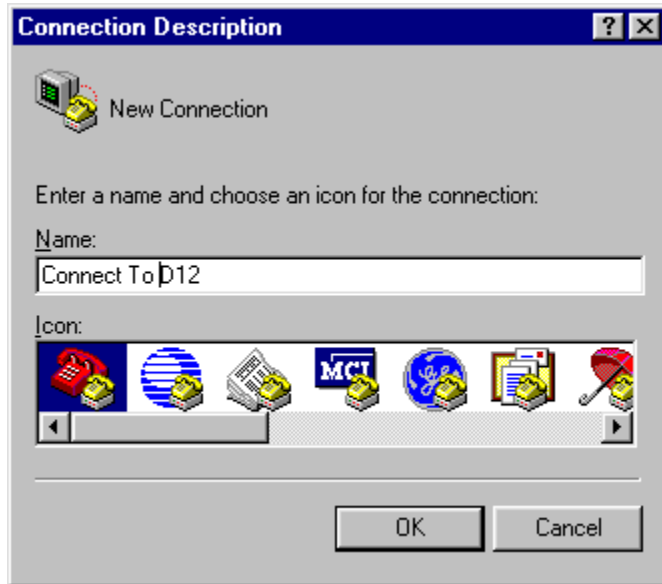


When the **Connect To** dialog appears, set **Connect using:** to **Direct to Com1** (or Direct to Com2 if you are using COM2) and click **OK**.



When the **COM1 Properties** dialog box appears, configure the Port Settings as shown below and click **OK**.

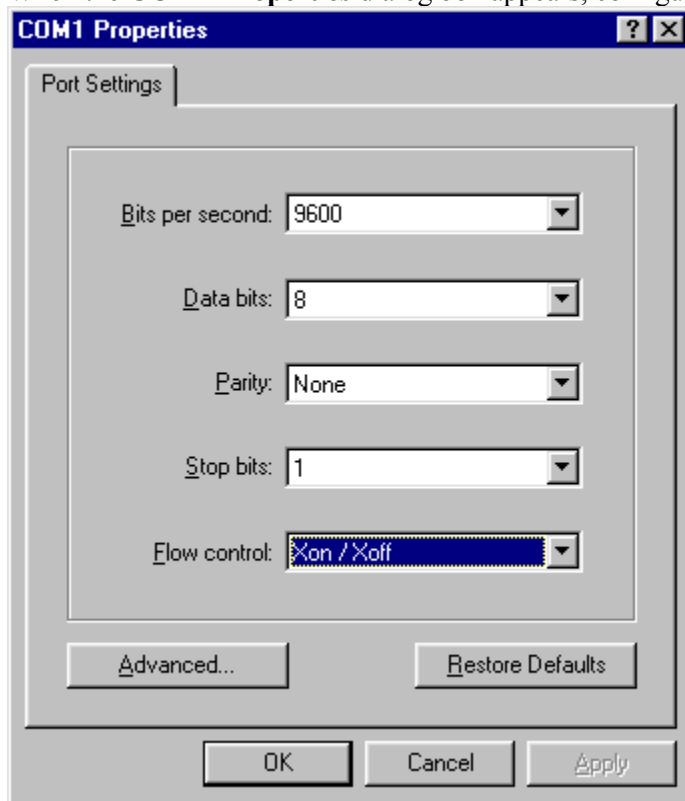


Click **View**, then click **Font** and configure the font settings as shown. This will insure that the data is presented in the terminal window without wrapping from line to line. You may need to experiment with these settings to obtain an acceptable presentation in the terminal window.

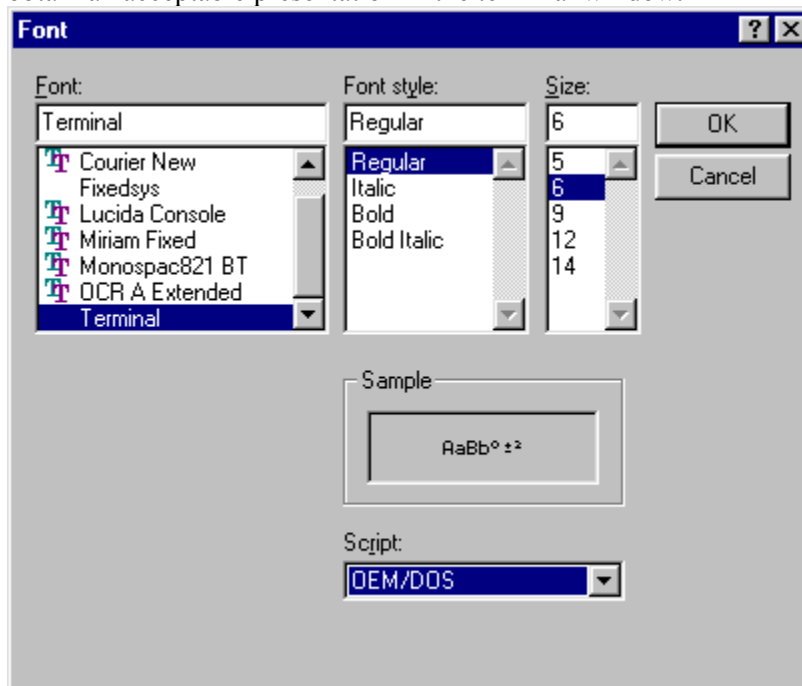


Click **OK** when finished.

**Series EXP-SNR Gas Transmitter with IR Sensor**


Click **File**, then click **Save As**, and click the **Save** button to store the settings as a HyperTerminal session file named Connect To D12.ht (the filename should automatically appear). You may later place this file on your desktop and simply click it to get this point automatically.

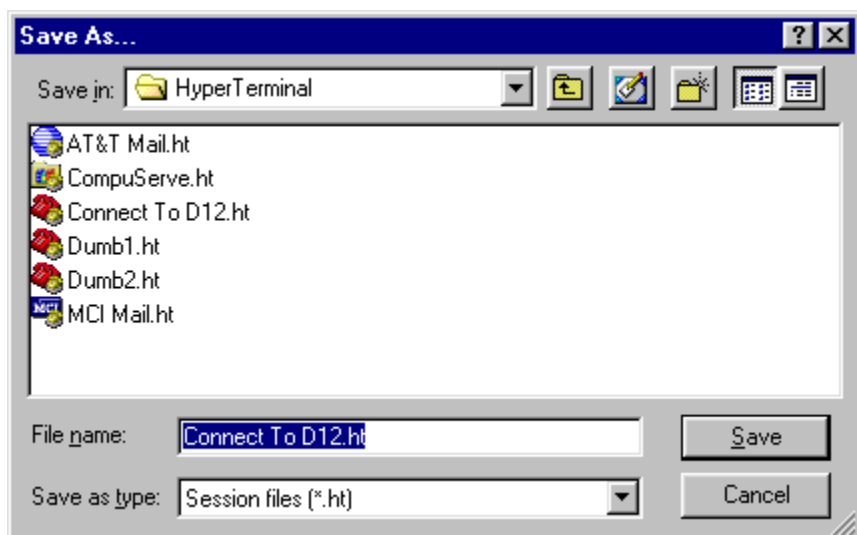

In order to chart the report data, it must be “captured” in a file and given a name. Click **Transfer** on the menu bar, click **Capture Text**, and then click the **Browse** button. Navigate to a folder and type the name of a file to store the report in (or choose an existing file to append the new report).

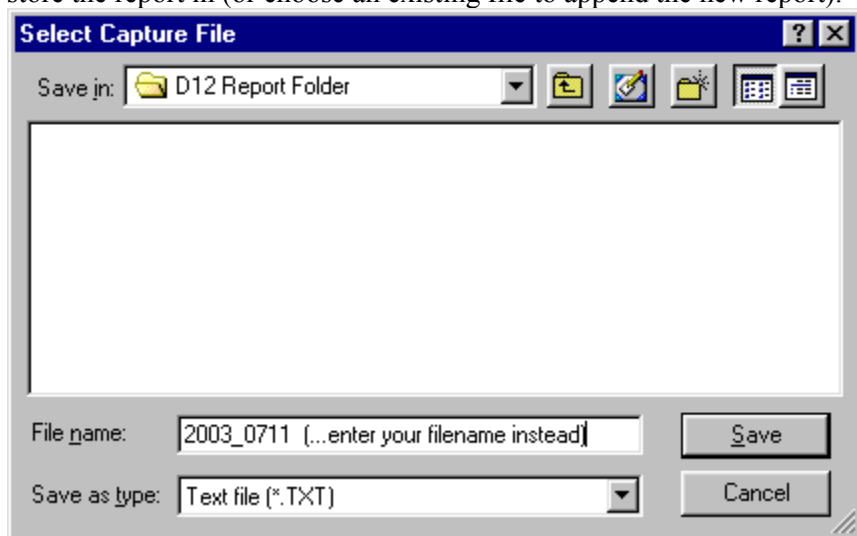


Click the **Save** button to return to the **Capture Text** dialog box. When the **Capture Text** dialog box reappears, click the **Start** button.

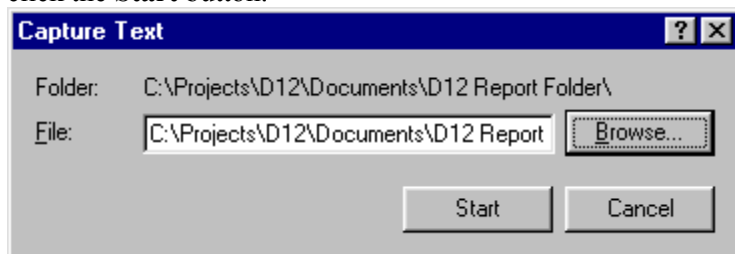

### Series EXP-SNR Gas Transmitter with IR Sensor

HyperTerminal is now ready to accept a report from the transmitter and save it in a file. Note that data may appear in the terminal window (shown below) if the Connect To D12 session has been run previously, but this data will not appear in the file just opened.

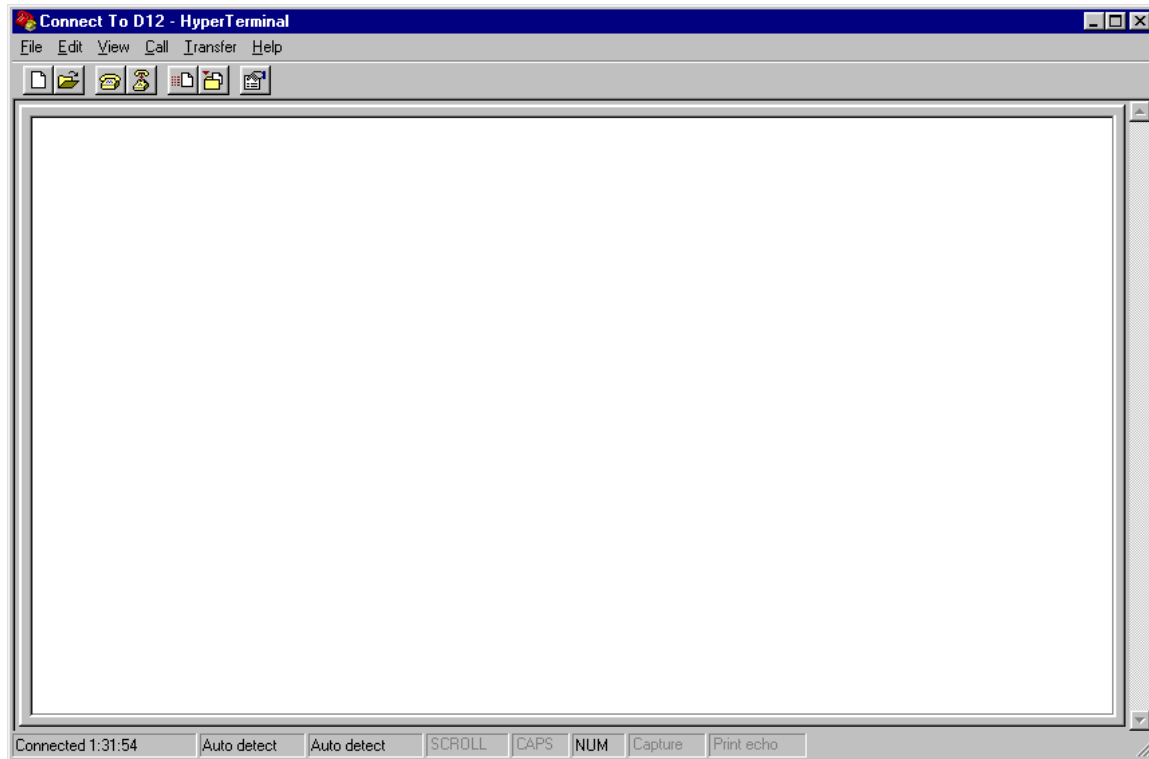

### **Starting the Report**

Prior to sending a report to the computer, the system clock should be set and the data logger turned on to record at least one sample. In addition, the Log\_Data variable (in the Menu/Setup/Auto-T/Setup menu) should be set to NO if you prefer to see the symbol TEST and not gas concentration values during auto-test.


Configure the communication variables as shown below. Note that 9600 is the highest baud rate common to the EXP-SNR transmitter and the Hyperterminal program.

Menu>Setup>System>Commun


```
►Protocol=ASCII
Interface=RS232
Baud_Rate=9600
Paramtrs=N,8,1
```

**Series EXP-SNR Gas Transmitter with IR Sensor**


Navigate to the DataLog page and select Print. You will not be allowed access if there are no samples in the log.

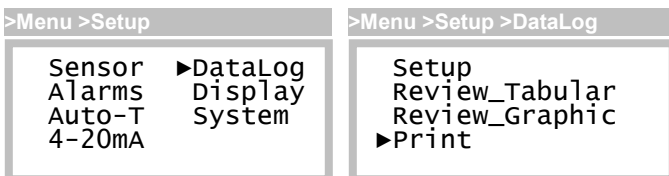


Select the first (starting) date. This will automatically re-compute the maximum number of days shown of the report (variable values will most likely differ from yours).

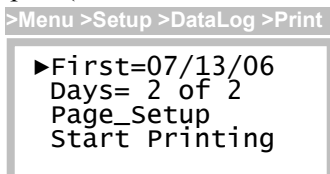


Edit the Days variable if you prefer to reduce the length of the report, otherwise the entire report will be printed.

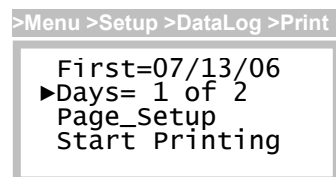

Select Page\_Setup and configure the Width, Eol, and EolDly variables as shown. The Width variable controls the number of sample columns printed and is settable from 1 to 30. Since the Hyperterminal display is 80 characters wide, set this to 10 columns so that data does not wrap around to the next line. Set Eol for CR/LF, and EolDly to 0.

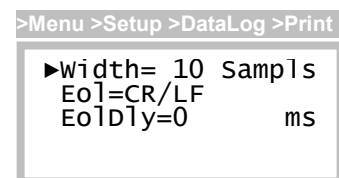


Escape from Page\_Setup and select Start\_Printing. "Printing" will begin flashing, and you may stop at any time by touching the Esc key.

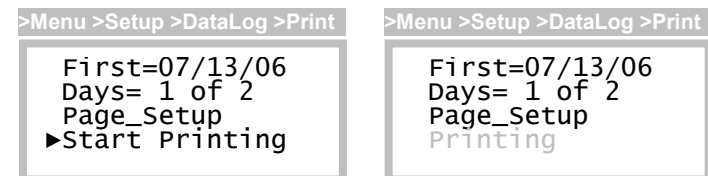

**Series EXP-SNR Gas Transmitter with IR Sensor**

The HyperTerminal terminal window should now begin to fill with lines from the report.

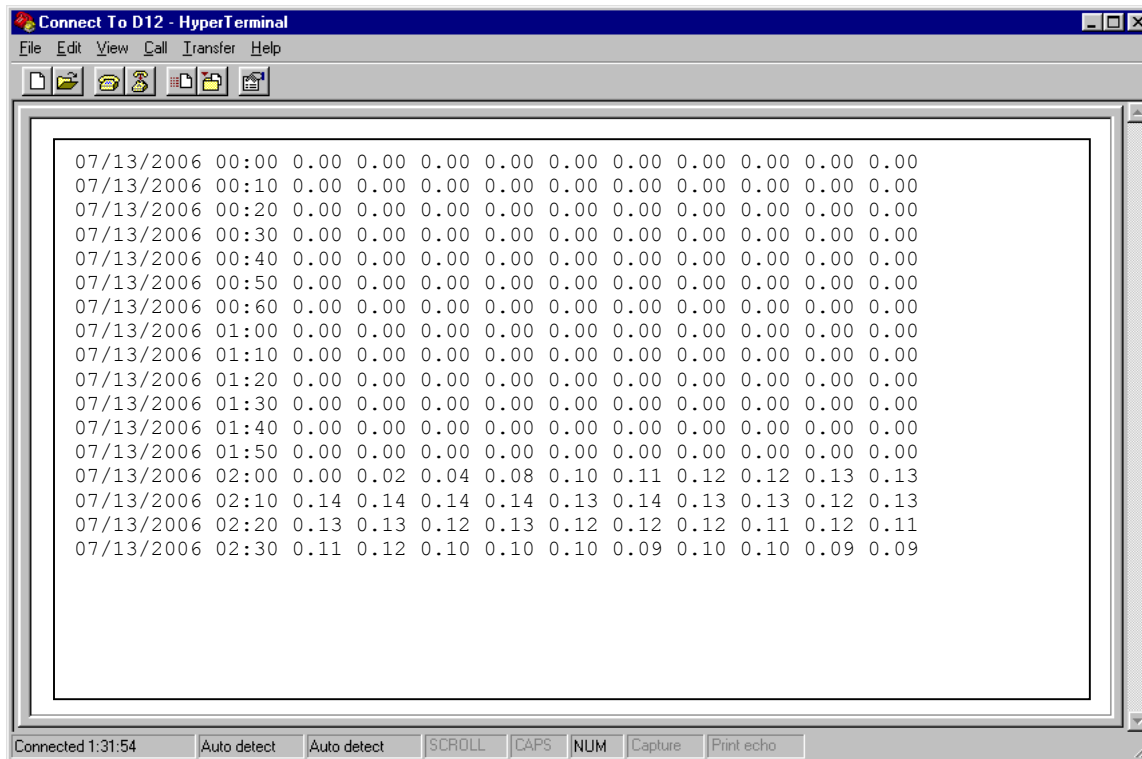

When the transmitter has stopped printing (displays Start\_Printing), click **Transfer**, move down to **Capture Text** and click **Stop**. This will close the report file so that it may be opened by another program.

## **Charting with Microsoft Excel**

Microsoft Excel can be used to import data log reports and create useful and informative charts.

Start Excel by clicking **Start**, pointing to **Programs**, and clicking **Microsoft Excel**.

When Excel opens, click **File** and then click **Open**. Navigate to the data log report file you wish to chart and click **Open**. Excel will recognize the report as a text file and offer some configuration options.

When the **Text Import Wizard – Step 1 of 3** appears, configure the settings as shown below and click **Next**. (Note that the values in your report file will be different than those shown below.)

**Text Import Wizard - Step 1 of 3**

The Text Wizard has determined that your data is Fixed Width.  
If this is correct, choose Next, or choose the data type that best describes your data.

Original data type

Choose the file type that best describes your data:

☒ **Delimited** - Characters such as commas or tabs separate each field.

☐ **Fixed width** - Fields are aligned in columns with spaces between each field.


Start import at row:  File origin:

Preview of file C:\Projects\D12\Documents\D12 Re...\2003\_0714.TXT.

|   |          |       |      |      |      |      |      |      |      |      |      |      |
|---|----------|-------|------|------|------|------|------|------|------|------|------|------|
| 1 | 07/13/03 | 00:00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 2 | 07/13/03 | 00:10 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 3 | 07/13/03 | 00:20 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 4 | 07/13/03 | 00:30 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 5 | 07/13/03 | 00:40 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |

Buttons: Cancel, < Back, Next >, Finish

When the **Text Import Wizard – Step 2 of 3** appears, configure the settings as shown below and click **Next**.

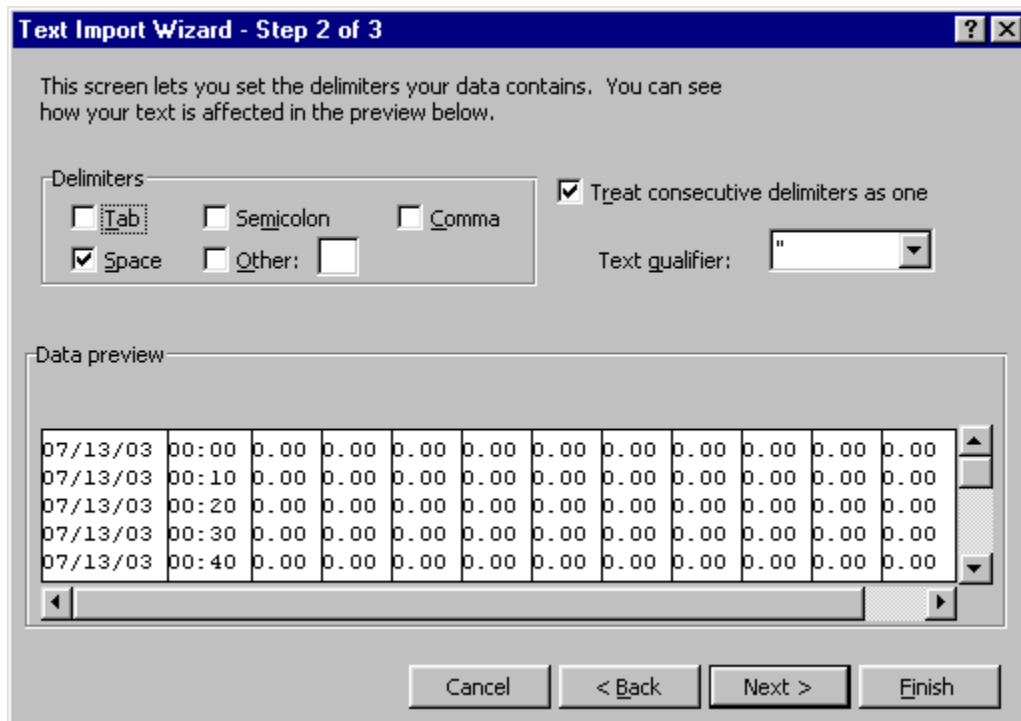

**Text Import Wizard - Step 2 of 3**

This screen lets you set the delimiters your data contains. You can see how your text is affected in the preview below.

**Delimiters**

☐ Tab    ☐ Semicolon    ☐ Comma  
☒ Space    ☐ Other:

☒ Treat consecutive delimiters as one


Text qualifier:

**Data preview**

|          |       |      |      |      |      |      |      |      |      |      |      |      |
|----------|-------|------|------|------|------|------|------|------|------|------|------|------|
| 07/13/03 | 00:00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 07/13/03 | 00:10 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 07/13/03 | 00:20 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 07/13/03 | 00:30 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |
| 07/13/03 | 00:40 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 | 0.00 |

Buttons: Cancel, < Back, Next >, Finish

When the **Text Import Wizard – Step 3 of 3** appears, click **Finish**.

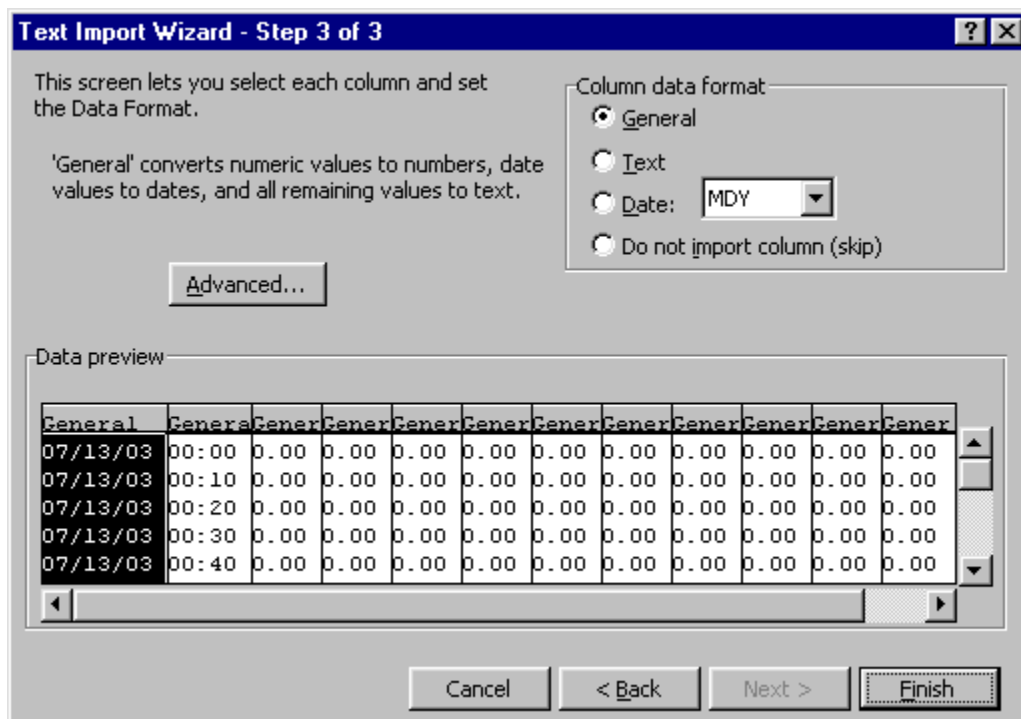

**Text Import Wizard - Step 3 of 3**

This screen lets you select each column and set the Data Format.

'General' converts numeric values to numbers, date values to dates, and all remaining values to text.

Advanced...

**Column data format:**

☒ General  
☐ Text  
☐ Date:   
☐ Do not import column (skip)

**Data preview**

| General  | General | General | General | General | General | General | General | General | General | General | General | General |
|----------|---------|---------|---------|---------|---------|---------|---------|---------|---------|---------|---------|---------|
| 07/13/03 | 00:00   | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    |
| 07/13/03 | 00:10   | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    |
| 07/13/03 | 00:20   | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    |
| 07/13/03 | 00:30   | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    |
| 07/13/03 | 00:40   | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    | 0.00    |

Buttons: Cancel, < Back, Next >, Finish

**Series EXP-SNR Gas Transmitter with IR Sensor**

The report should appear as a spreadsheet resembling the format shown below. Of course the dates, times, and values will be different.

|    | A     | B    | C | D | E | F | G | H | I | J | K | L | M | N | O | P | Q |
|----|-------|------|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|
| 1  | SNR13 | 0.00 | C | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 2  | EXP11 | 0.00 | C | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 3  | SNR13 | 0.00 | C | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 4  | EXP11 | 0.00 | C | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 5  | SNR13 | 0.00 | C | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 6  | EXP11 | 0.00 | C | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 7  | SNR13 | 0.00 | C | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 8  | EXP11 | 0.00 | C | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 9  | SNR13 | 0.00 | C | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 10 | EXP11 | 0.00 | C | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 11 | SNR13 | 0.00 | C | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 12 | EXP11 | 0.00 | C | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 13 | SNR13 | 0.00 | C | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 14 | EXP11 | 0.00 | C | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 15 | SNR13 | 0.00 | C | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 16 | EXP11 | 0.00 | C | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 17 | SNR13 | 0.00 | C | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 18 | EXP11 | 0.00 | C | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 19 | SNR13 | 0.00 | C | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 20 | EXP11 | 0.00 | C | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 21 | SNR13 | 0.00 | C | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 22 | EXP11 | 0.00 | C | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |

### **Series EXP-SNR Gas Transmitter with IR Sensor**

To chart the report, select one full day of data by dragging the mouse cursor over the region to be charted. Notice that this region begins in the time of day column and extends across each of the sample columns.

Microsoft Excel 2003 0714 7

File Edit View Insert Format Tools Data Window Help

Format Cells | Font | Number | Styles | Window | Help


Sum: 100.000000

|    | A         | B    | C | D | E | F | G | H | I | J | K | L | M | N | O |
|----|-----------|------|---|---|---|---|---|---|---|---|---|---|---|---|---|
| 1  | 7/1/2003  | 0.00 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 2  | 7/2/2003  | 0.00 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 3  | 7/3/2003  | 0.00 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 4  | 7/4/2003  | 0.00 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 5  | 7/5/2003  | 0.00 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 6  | 7/6/2003  | 0.00 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 7  | 7/7/2003  | 0.00 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 8  | 7/8/2003  | 0.00 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 9  | 7/9/2003  | 0.00 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 10 | 7/10/2003 | 0.00 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 11 | 7/11/2003 | 0.00 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 12 | 7/12/2003 | 0.00 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 13 | 7/13/2003 | 0.00 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 14 | 7/14/2003 | 0.00 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 15 | 7/15/2003 | 0.00 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 16 | 7/16/2003 | 0.00 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 17 | 7/17/2003 | 0.00 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 18 | 7/18/2003 | 0.00 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 19 | 7/19/2003 | 0.00 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 20 | 7/20/2003 | 0.00 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 21 | 7/21/2003 | 0.00 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 22 | 7/22/2003 | 0.00 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 23 | 7/23/2003 | 0.00 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 24 | 7/24/2003 | 0.00 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 25 | 7/25/2003 | 0.00 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 26 | 7/26/2003 | 0.00 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 27 | 7/27/2003 | 0.00 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 28 | 7/28/2003 | 0.00 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 29 | 7/29/2003 | 0.00 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 30 | 7/30/2003 | 0.00 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 31 | 7/31/2003 | 0.00 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |
| 32 | 7/32/2003 | 0.00 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |

Sum: 100.000000


After selecting the region, click Insert and then Chart (or click the Chart icon directly from the toolbar).

When the **Chart Type** dialog appears, click on **Column**, and click **Next**.

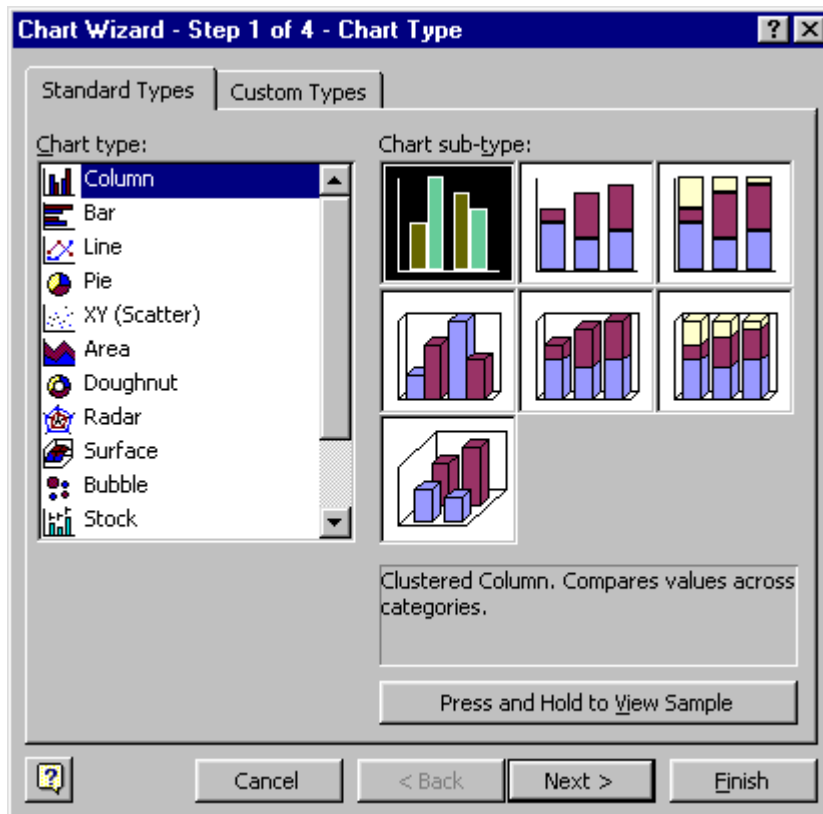


**Series EXP-SNR Gas Transmitter with IR Sensor**


When the **Chart Source Data** dialog appears, click **Next**.

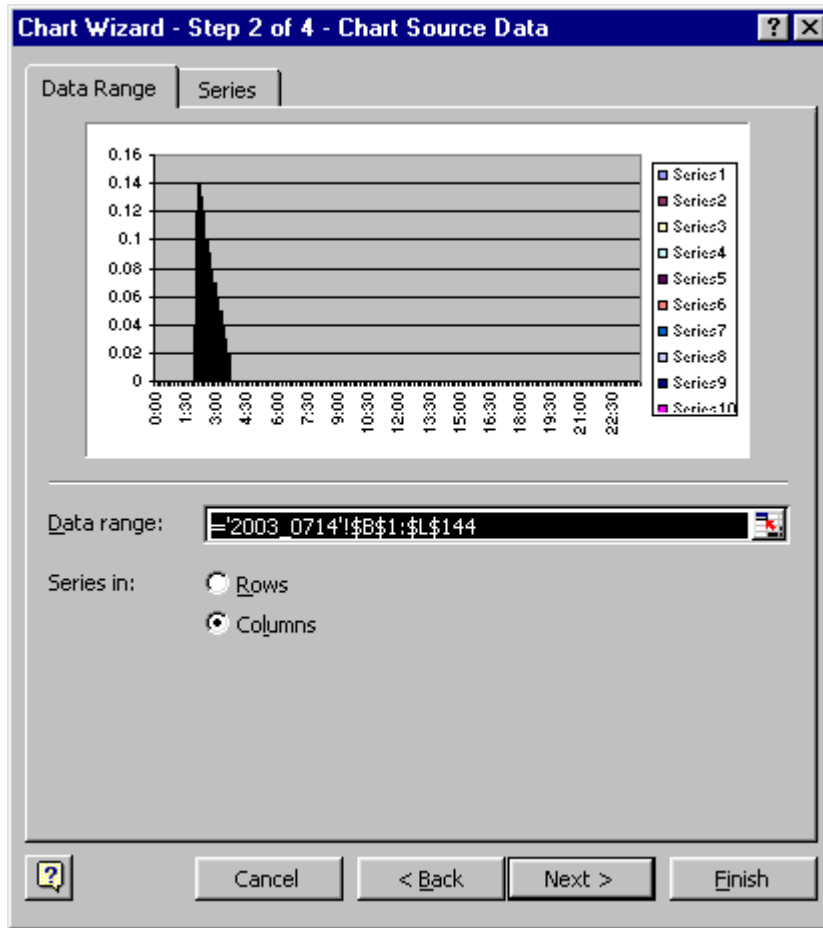

When the **Chart Options** dialog appears, click off the **Show legend** option, and click **Next**.

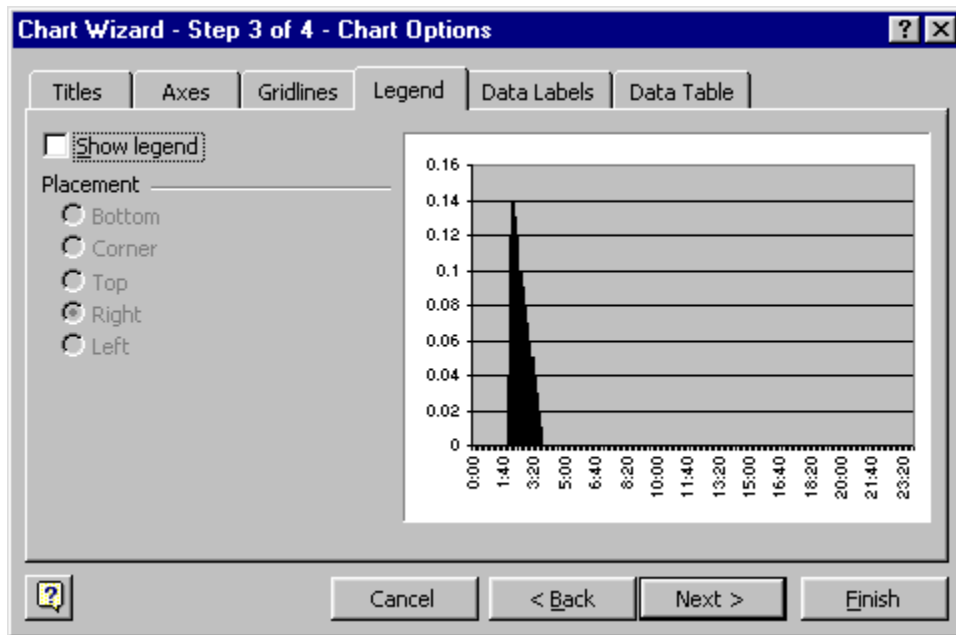


When the **Chart Location** dialog appears, click the **As new sheet** radio button and enter the name of a new sheet to store the chart in. Alternately, you may click the **As object in** radio button to place the chart onto the sheet you have just created.

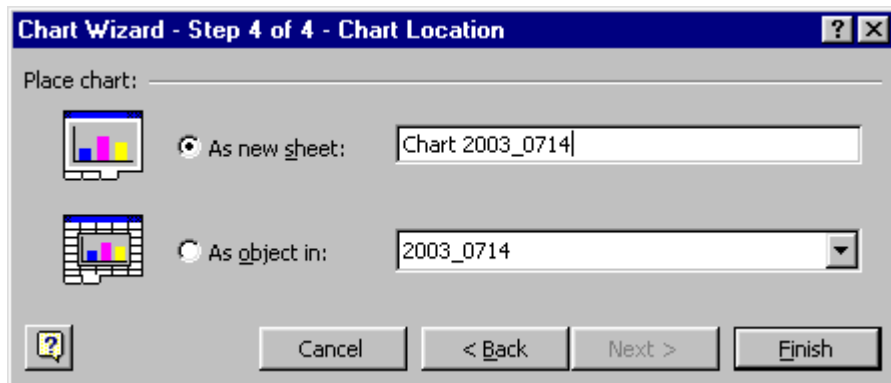


**Series EXP-SNR Gas Transmitter with IR Sensor**

If you have previously clicked the **As new sheet** radio button, the chart will appear on the new sheet named above. You may now move between the new sheet and the old sheet by clicking the sheet tabs that appear just below the chart display.

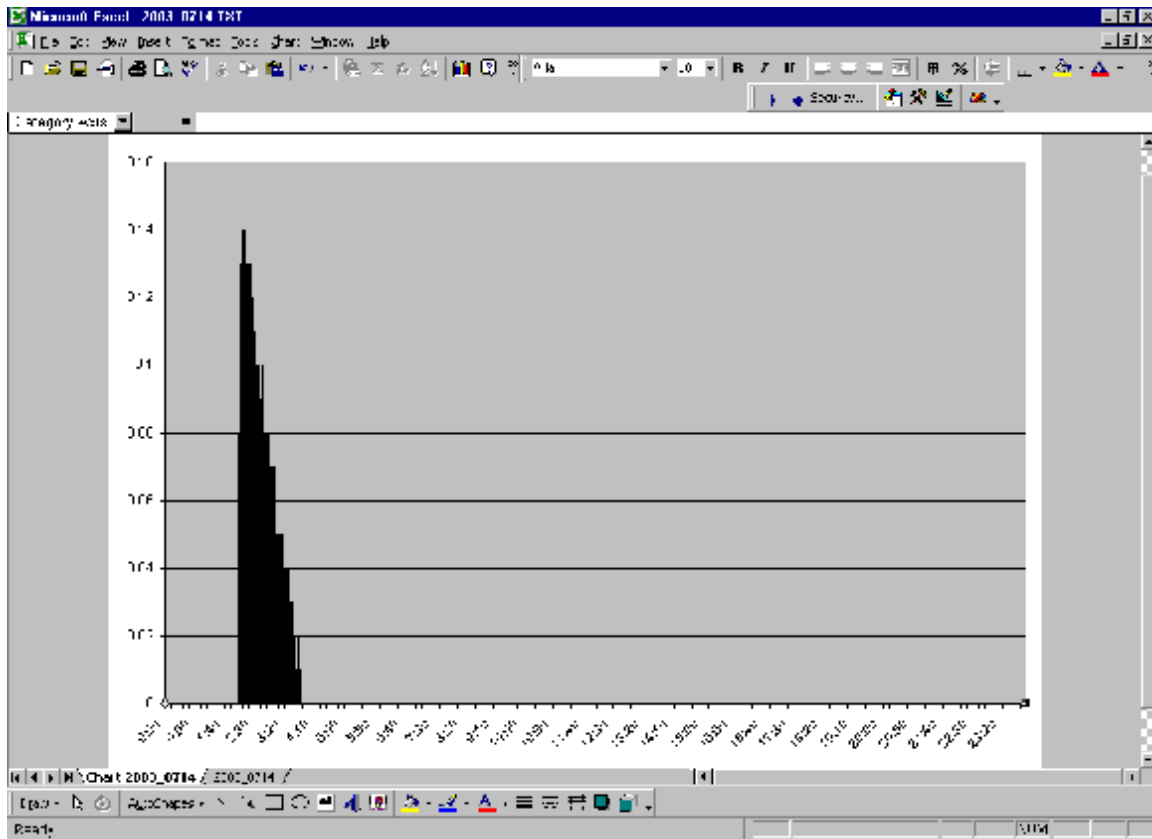

### Series EXP-SNR Gas Transmitter with IR Sensor

If you have previously clicked the **As object in:** radio button, the chart will appear on the existing sheet.

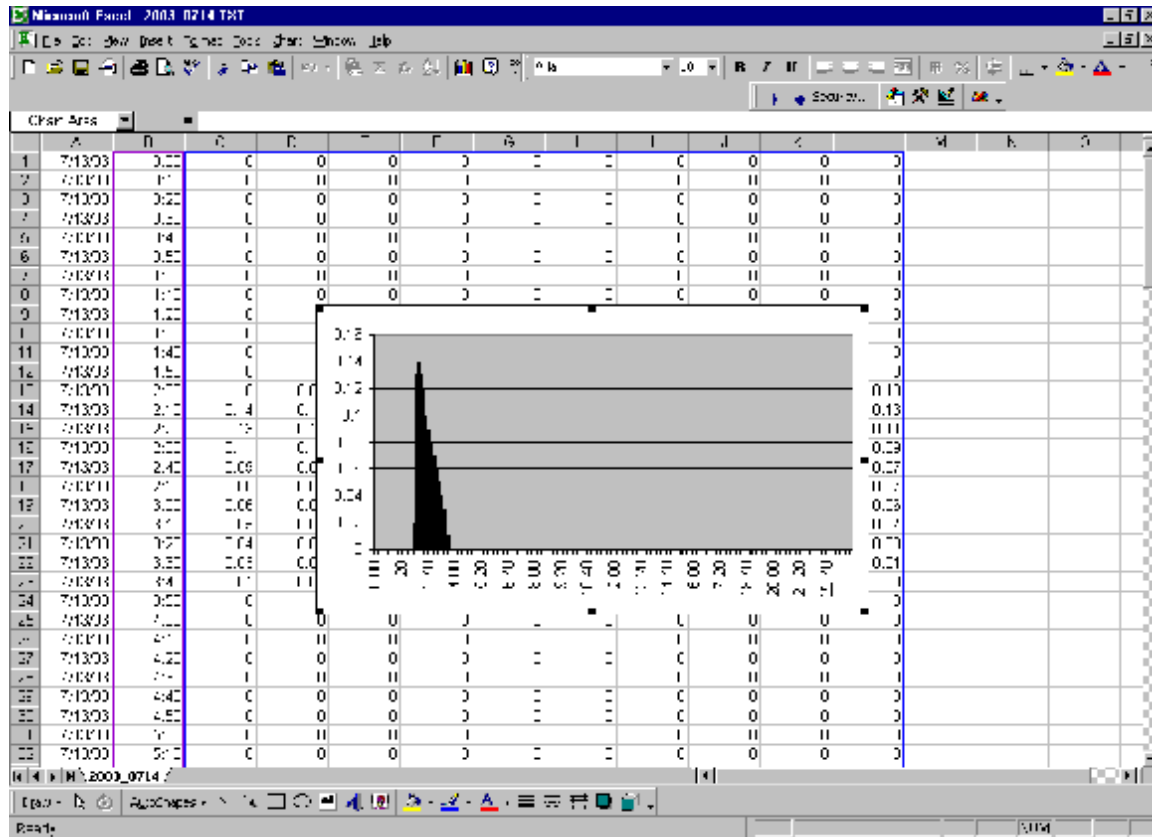

Finally, click **File**, then **Save** to store the chart.

Once the chart has been created, you may wish to rescale it, title it, and print it. These features are detailed in Microsoft Excel Help and are beyond the scope of this document.